

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007157.D
 Acq On : 23 Aug 2018 22:37
 Operator : SY/MD
 Sample : J4622-15
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK7

Quant Time: Aug 24 02:55:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 02:07:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	540768	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	518504	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	185723	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	142279	41.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.74%
7) Chloroethane-d5	1.57	69	123766	56.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	113.26%
11) 1,1-Dichloroethene-d2	2.13	63	204849	32.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.10%
21) 2-Butanone-d5	3.95	46	284223	98.27	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.27%
24) Chloroform-d	4.41	84	340236	46.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.09	65	216138	49.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.06%
32) Benzene-d6	5.10	84	670717	46.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.08%
36) 1,2-Dichloropropane-d6	6.12	67	229050	48.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.10%
41) Toluene-d8	7.37	98	515055	40.62	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.24%
43) trans-1,3-Dichloropropene-	7.67	79	85046	41.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.34%
47) 2-Hexanone-d5	8.14	63	120759	71.24	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	71.24%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	309206	44.59	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.18%
64) 1,2-Dichlorobenzene-d4	11.68	152	189299	50.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.38%


Target Compounds					Ovalue
13) Acetone	2.20	43	10139	4.47 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082318\
Data File : VV007157.D
Acq On : 23 Aug 2018 22:37
Operator : SY/MD
Sample : J4622-15
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBK7

Quant Time: Aug 24 02:55:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 02:07:07 2018
Response via : Initial Calibration

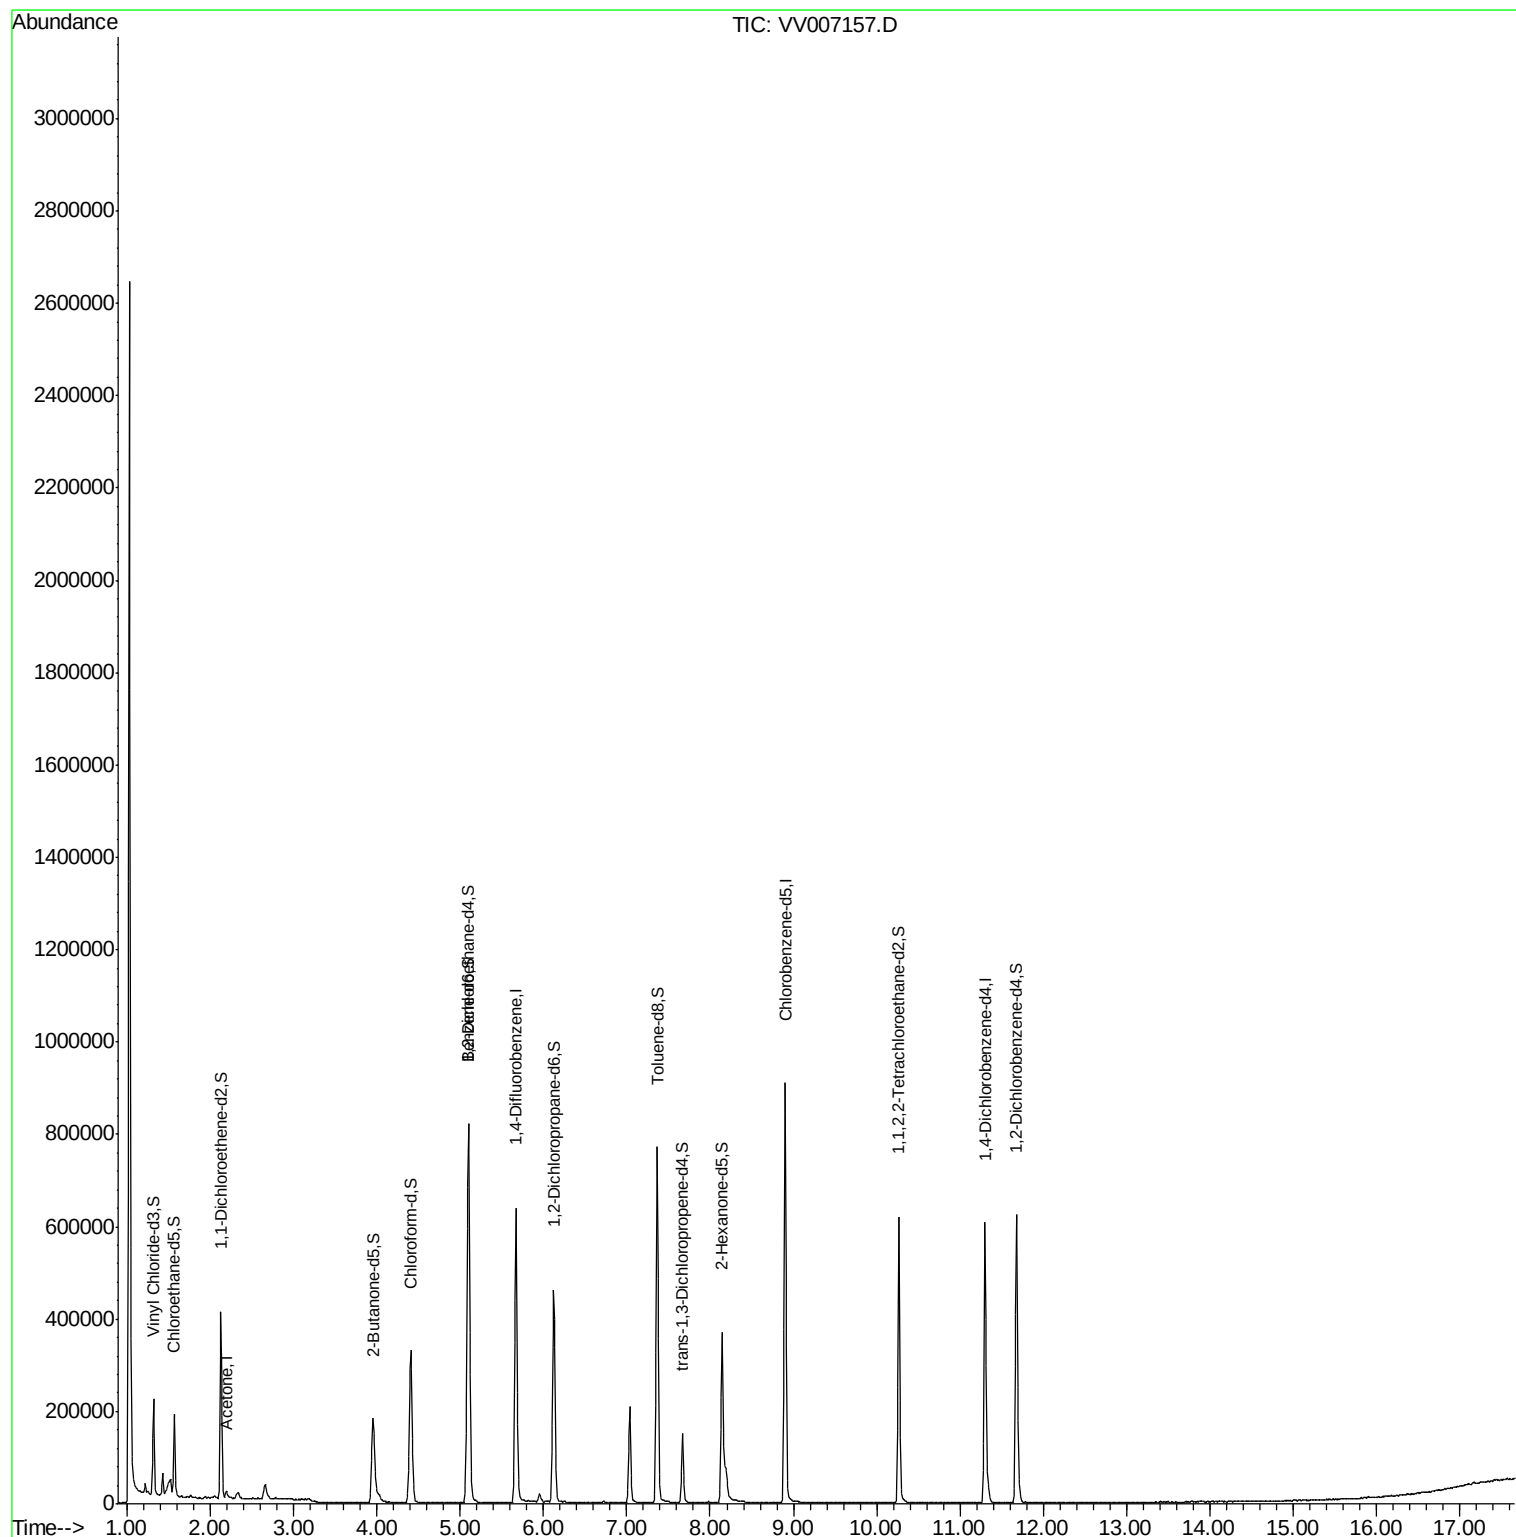

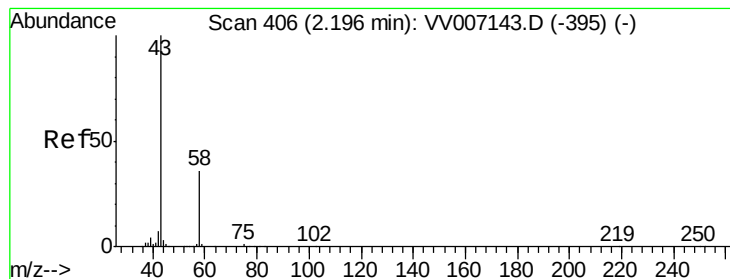

#13
 Acetone
 Concen: 4.47 ug/L
 RT: 2.20 min Scan# 406
 Delta R.T. 0.00 min
 Lab File: VV007157.D
 Acq: 23 Aug 2018 22:37

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK7

Tot Ion: 43 Resp: 10139
 Ion Ratio Lower Upper
 43 100
 58 35.7 0.0 73.0

