

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007130.D
 Acq On : 23 Aug 2018 10:15
 Operator : SY/MD
 Sample : VV0823WBL01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.922	6	10	12	rBV2	511	436	0.01%	0.002%
2	0.964	21	23	26	rBV3	587	423	0.01%	0.002%
3	1.032	30	44	67	rBV	2152551	2962624	100.00%	15.364%
4	1.321	126	134	151	rVB	269713	299646	10.11%	1.554%
5	1.578	208	214	231	rVB	233926	280073	9.45%	1.452%
6	2.131	376	386	398	rBV	515668	720024	24.30%	3.734%
7	3.305	749	751	754	rBV2	947	719	0.02%	0.004%
8	3.601	840	843	845	rBV3	650	472	0.02%	0.002%
9	3.672	862	865	871	rBV5	702	625	0.02%	0.003%
10	3.958	937	954	996	rBV	186288	608081	20.53%	3.153%
11	4.405	1074	1093	1119	rBV	381454	919027	31.02%	4.766%
12	4.588	1147	1150	1157	rVB7	1044	1108	0.04%	0.006%
13	4.668	1171	1175	1177	rBV3	795	677	0.02%	0.004%
14	4.723	1187	1192	1199	rVV8	1553	2362	0.08%	0.012%
15	4.781	1208	1210	1216	rVB4	894	715	0.02%	0.004%
16	4.813	1216	1220	1221	rBV4	684	524	0.02%	0.003%
17	5.000	1275	1278	1285	rVB5	594	667	0.02%	0.003%
18	5.035	1285	1289	1290	rBV3	794	521	0.02%	0.003%
19	5.099	1290	1309	1350	rBV2	966280	2337473	78.90%	12.122%
20	5.321	1376	1378	1384	rVB3	716	536	0.02%	0.003%
21	5.392	1398	1400	1407	rVB4	907	962	0.03%	0.005%
22	5.427	1409	1411	1414	rBV2	1038	664	0.02%	0.003%
23	5.450	1417	1418	1422	rVB4	1123	602	0.02%	0.003%
24	5.508	1434	1436	1441	rVB4	1111	678	0.02%	0.004%
25	5.610	1465	1468	1470	rBV3	828	523	0.02%	0.003%
26	5.668	1470	1486	1511	rBV	686606	1384518	46.73%	7.180%
27	5.951	1566	1574	1588	rVB8	15161	31081	1.05%	0.161%
28	6.122	1611	1627	1659	rBV	531527	1073216	36.23%	5.566%
29	6.527	1749	1753	1758	rVV5	824	722	0.02%	0.004%
30	6.559	1758	1763	1766	rVB4	634	591	0.02%	0.003%
31	6.643	1786	1789	1791	rBV3	676	472	0.02%	0.002%
32	6.700	1802	1807	1808	rBV3	880	738	0.02%	0.004%
33	6.713	1808	1811	1814	rVV3	931	934	0.03%	0.005%
34	6.823	1840	1845	1850	rBV5	1087	1033	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007130.D
 Acq On : 23 Aug 2018 10:15
 Operator : SY/MD
 Sample : VV0823WBL01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

35	6.897	1866	1868	1873	rVB2	887	546	0.02%	0.003%
36	6.980	1891	1894	1896	rVB3	772	423	0.01%	0.002%
37	7.035	1896	1911	1929	rBV	247751	448900	15.15%	2.328%
38	7.253	1975	1979	1980	rBV2	1091	579	0.02%	0.003%
39	7.292	1984	1991	1994	rVV4	1840	2223	0.08%	0.012%
40	7.363	1999	2013	2033	rBV	942350	1662386	56.11%	8.621%
41	7.668	2096	2108	2125	rBV	172360	293652	9.91%	1.523%
42	7.794	2143	2147	2148	rBV3	1308	780	0.03%	0.004%
43	7.890	2174	2177	2179	rBV5	1257	800	0.03%	0.004%
44	8.022	2213	2218	2224	rVB5	2477	3520	0.12%	0.018%
45	8.051	2224	2227	2229	rVB2	822	515	0.02%	0.003%
46	8.141	2243	2255	2295	rBV2	422470	985178	33.25%	5.109%
47	8.485	2360	2362	2367	rVB3	980	634	0.02%	0.003%
48	8.511	2367	2370	2371	rBV3	770	408	0.01%	0.002%
49	8.633	2405	2408	2411	rVB3	641	441	0.01%	0.002%
50	8.732	2437	2439	2442	rVB2	716	429	0.01%	0.002%
51	8.787	2453	2456	2460	rVB4	798	507	0.02%	0.003%
52	8.810	2460	2463	2469	rBV5	912	796	0.03%	0.004%
53	8.900	2477	2491	2520	rBV	978024	1609301	54.32%	8.346%
54	9.048	2534	2537	2538	rBV3	1997	1179	0.04%	0.006%
55	9.192	2574	2582	2594	rVB8	2948	5418	0.18%	0.028%
56	9.337	2623	2627	2632	rVB4	1040	698	0.02%	0.004%
57	9.379	2637	2640	2644	rVV4	900	535	0.02%	0.003%
58	9.411	2648	2650	2655	rVB2	784	499	0.02%	0.003%
59	9.443	2655	2660	2662	rBV4	777	673	0.02%	0.003%
60	9.495	2673	2676	2680	rBV3	731	527	0.02%	0.003%
61	9.610	2701	2712	2721	rVB10	2736	5732	0.19%	0.030%
62	9.646	2721	2723	2728	rVB5	874	666	0.02%	0.003%
63	9.675	2728	2732	2734	rBV3	986	746	0.03%	0.004%
64	9.691	2734	2737	2743	rVB4	546	565	0.02%	0.003%
65	9.781	2761	2765	2770	rBV4	606	730	0.02%	0.004%
66	9.935	2807	2813	2816	rVV5	636	736	0.02%	0.004%
67	9.983	2820	2828	2838	rBV4	2929	4819	0.16%	0.025%
68	10.028	2838	2842	2845	rBV3	688	640	0.02%	0.003%
69	10.170	2880	2886	2889	rBV3	898	809	0.03%	0.004%
70	10.266	2904	2916	2933	rBV	667809	1078200	36.39%	5.592%
71	10.536	2994	3000	3005	rVB4	892	1178	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007130.D
 Acq On : 23 Aug 2018 10:15
 Operator : SY/MD
 Sample : VV0823WBL01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

72	10.565	3005	3009	3012	rBV3	756	665	0.02%	0.003%
73	10.649	3031	3035	3037	rVV3	497	477	0.02%	0.002%
74	10.691	3046	3048	3050	rVV2	737	459	0.02%	0.002%
75	10.713	3053	3055	3060	rVB4	1098	684	0.02%	0.004%
76	10.867	3099	3103	3109	rVB4	1023	834	0.03%	0.004%
77	10.900	3110	3113	3116	rBV2	931	632	0.02%	0.003%
78	10.935	3119	3124	3127	rBV3	585	471	0.02%	0.002%
79	10.967	3132	3134	3139	rVB4	719	550	0.02%	0.003%
80	10.999	3139	3144	3146	rVB4	566	429	0.01%	0.002%
81	11.195	3202	3205	3208	rBV3	573	427	0.01%	0.002%
82	11.231	3211	3216	3224	rVV7	3639	4624	0.16%	0.024%
83	11.302	3224	3238	3264	rVV	664630	1189506	40.15%	6.169%
84	11.459	3284	3287	3288	rBV2	819	448	0.02%	0.002%
85	11.469	3288	3290	3296	rVB5	953	801	0.03%	0.004%
86	11.678	3342	3355	3378	rBV	757695	1314010	44.35%	6.814%
87	11.996	3450	3454	3455	rBV2	616	445	0.02%	0.002%
88	12.086	3480	3482	3486	rVB4	905	607	0.02%	0.003%
89	12.112	3486	3490	3493	rVB3	586	482	0.02%	0.002%
90	12.314	3550	3553	3555	rBV4	715	522	0.02%	0.003%
91	12.504	3610	3612	3615	rBV3	595	454	0.02%	0.002%
92	12.832	3712	3714	3718	rBV4	892	527	0.02%	0.003%
93	12.986	3759	3762	3765	rBV2	1074	657	0.02%	0.003%
94	13.025	3772	3774	3778	rBV3	954	688	0.02%	0.004%
95	13.318	3862	3865	3874	rVB7	3809	4763	0.16%	0.025%
96	13.356	3875	3877	3881	rVB5	1019	484	0.02%	0.003%
97	13.803	4010	4016	4026	rBV8	3442	5712	0.19%	0.030%
98	13.909	4047	4049	4052	rBV3	1412	654	0.02%	0.003%
99	14.018	4080	4083	4087	rBV4	1298	808	0.03%	0.004%
100	14.044	4087	4091	4095	rBV5	1002	1080	0.04%	0.006%


Sum of corrected areas: 19282735

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082318\
Data File : VV007130.D
Acq On : 23 Aug 2018 10:15
Operator : SY/MD
Sample : VV0823WBL01
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK61

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

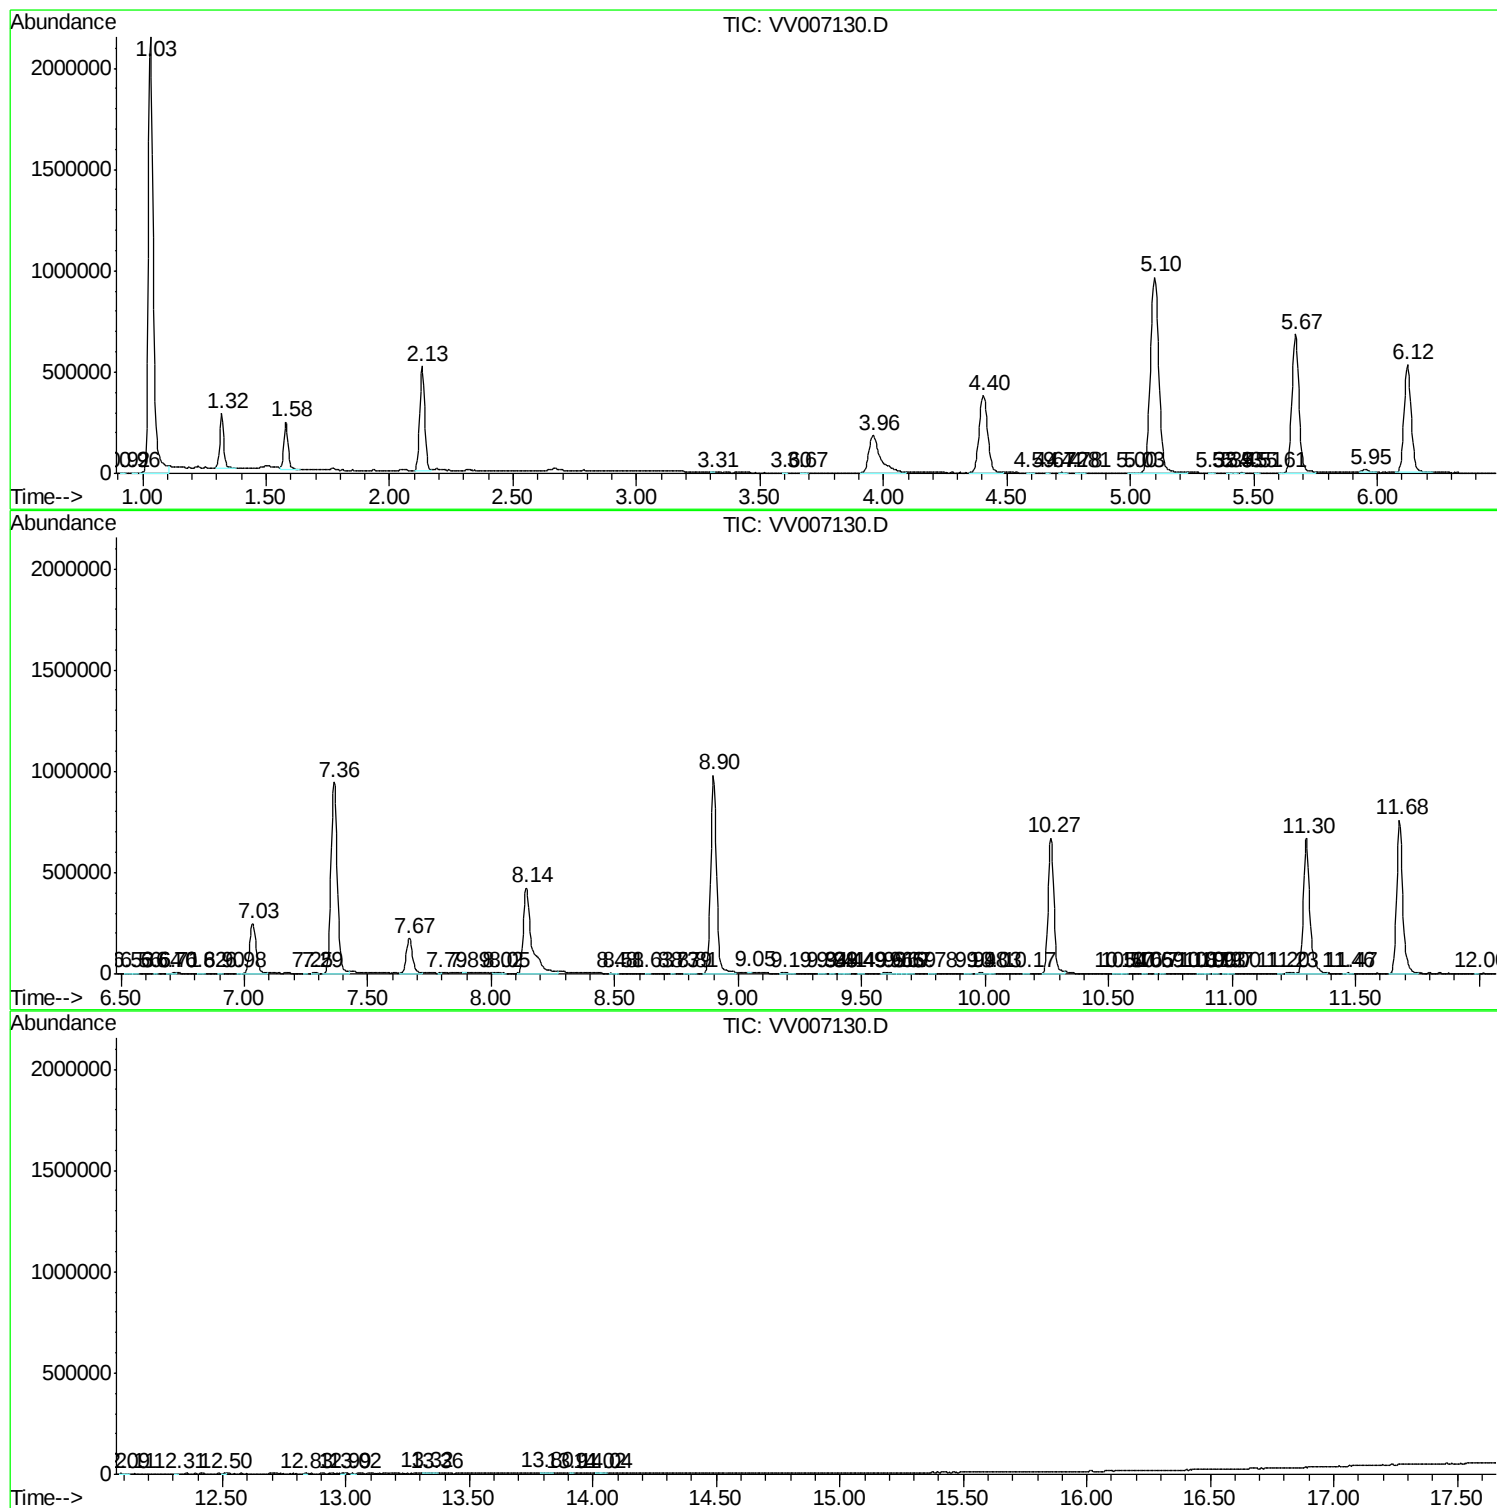

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082318\
Data File : VV007130.D
Acq On : 23 Aug 2018 10:15
Operator : SY/MD
Sample : VV0823WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK61

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082318\
Data File : VV007130.D
Acq On : 23 Aug 2018 10:15
Operator : SY/MD
Sample : VV0823WBL01
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK61

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc