

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007134.D
 Acq On : 23 Aug 2018 12:39
 Operator : SY/MD
 Sample : J4599-02 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETOK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.945	12	17	19	rBV2	779	754	0.002%	0.0004%
2	1.025	28	42	75	rBV	2461669	3249610	100.00%	15.970%
3	1.222	98	103	108	rBV	26897	25343	0.78%	0.125%
4	1.325	125	135	163	rBV2	1282565	1464109	45.05%	7.195%
5	1.556	203	207	230	rVB	180720	225948	6.95%	1.110%
6	2.125	374	384	396	rBV	403416	572260	17.61%	2.812%
7	3.562	825	831	834	rBV4	705	990	0.03%	0.0005%
8	3.582	835	837	842	rVB6	712	520	0.02%	0.0003%
9	3.649	854	858	863	rBV5	914	1122	0.03%	0.0006%
10	3.672	863	865	873	rVB3	956	839	0.03%	0.0004%
11	3.713	873	878	880	rBV3	715	580	0.02%	0.0003%
12	3.781	896	899	901	rBV4	561	337	0.01%	0.0002%
13	3.964	935	956	998	rBV2	1193853	3005686	92.49%	14.771%
14	4.308	1060	1063	1066	rVB3	1046	667	0.02%	0.0003%
15	4.324	1066	1068	1071	rVB3	1085	486	0.01%	0.0002%
16	4.405	1075	1093	1117	rVV	310159	738170	22.72%	3.628%
17	4.710	1184	1188	1189	rBV2	905	671	0.02%	0.0003%
18	4.755	1200	1202	1212	rVB5	1010	1191	0.04%	0.0006%
19	4.906	1247	1249	1251	rBV	581	396	0.01%	0.0002%
20	4.948	1259	1262	1268	rVB4	658	522	0.02%	0.0003%
21	4.977	1268	1271	1272	rBV	819	405	0.01%	0.0002%
22	5.012	1278	1282	1284	rBV4	589	435	0.01%	0.0002%
23	5.096	1290	1308	1343	rBV2	782601	1904266	58.60%	9.358%
24	5.302	1369	1372	1374	rBV3	596	332	0.01%	0.0002%
25	5.369	1389	1393	1394	rBV3	1005	672	0.02%	0.0003%
26	5.517	1438	1439	1442	rVV2	805	501	0.02%	0.0002%
27	5.668	1467	1486	1509	rBV	591641	1182246	36.38%	5.810%
28	5.951	1563	1574	1591	rVB3	18651	38948	1.20%	0.191%
29	6.122	1612	1627	1649	rBV	434381	871808	26.83%	4.284%
30	6.334	1691	1693	1698	rBV4	752	495	0.02%	0.0002%
31	6.717	1803	1812	1824	rBV3	6087	12126	0.37%	0.060%
32	6.839	1847	1850	1853	rBV5	887	712	0.02%	0.0003%
33	6.861	1855	1857	1860	rVB3	858	531	0.02%	0.0003%
34	6.887	1860	1865	1868	rBV3	1149	937	0.03%	0.0005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007134.D
 Acq On : 23 Aug 2018 12:39
 Operator : SY/MD
 Sample : J4599-02 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETOK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

35	7.035	1898	1911	1933	rBV	209744	374350	11.52%	1.840%
36	7.170	1949	1953	1961	rVB5	1362	1922	0.06%	0.009%
37	7.241	1973	1975	1979	rBV3	705	500	0.02%	0.002%
38	7.260	1979	1981	1984	rBV4	514	333	0.01%	0.002%
39	7.363	1999	2013	2030	rBV	756030	1312206	40.38%	6.449%
40	7.668	2097	2108	2123	rVV	148877	248212	7.64%	1.220%
41	7.813	2147	2153	2155	rBV6	1068	1067	0.03%	0.005%
42	7.942	2188	2193	2196	rBV5	1302	1156	0.04%	0.006%
43	8.144	2243	2256	2268	rBV	340864	689940	21.23%	3.391%
44	8.569	2386	2388	2390	rBV2	858	335	0.01%	0.002%
45	8.623	2402	2405	2409	rBV5	604	471	0.01%	0.002%
46	8.662	2412	2417	2419	rBV5	800	588	0.02%	0.003%
47	8.765	2446	2449	2453	rVV3	864	752	0.02%	0.004%
48	8.787	2453	2456	2462	rVV4	943	889	0.03%	0.004%
49	8.842	2469	2473	2476	rBV3	682	618	0.02%	0.003%
50	8.900	2476	2491	2521	rBV	831038	1373260	42.26%	6.749%
51	9.151	2567	2569	2573	rBV3	597	401	0.01%	0.002%
52	9.176	2574	2577	2579	rBV3	738	537	0.02%	0.003%
53	9.215	2587	2589	2593	rBV2	525	375	0.01%	0.002%
54	9.282	2606	2610	2613	rBV3	447	393	0.01%	0.002%
55	9.363	2631	2635	2636	rBV2	592	421	0.01%	0.002%
56	9.427	2647	2655	2656	rBV4	651	843	0.03%	0.004%
57	9.498	2673	2677	2681	rBV4	675	590	0.02%	0.003%
58	9.520	2681	2684	2688	rBV4	669	565	0.02%	0.003%
59	9.581	2694	2703	2704	rBV4	830	1050	0.03%	0.005%
60	9.681	2732	2734	2738	rBV3	513	346	0.01%	0.002%
61	9.742	2750	2753	2756	rBV2	540	406	0.01%	0.002%
62	9.803	2767	2772	2774	rBV2	1037	758	0.02%	0.004%
63	9.829	2777	2780	2784	rVV2	605	382	0.01%	0.002%
64	9.855	2784	2788	2794	rVB4	860	684	0.02%	0.003%
65	9.922	2806	2809	2813	rVB2	722	495	0.02%	0.002%
66	9.945	2813	2816	2819	rBV4	495	441	0.01%	0.002%
67	10.025	2836	2841	2845	rVB4	627	540	0.02%	0.003%
68	10.067	2849	2854	2858	rBV3	710	643	0.02%	0.003%
69	10.151	2875	2880	2884	rVB6	884	869	0.03%	0.004%
70	10.269	2900	2917	2952	rBV	573041	954226	29.36%	4.689%
71	10.395	2952	2956	2959	rBV2	776	589	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007134.D
 Acq On : 23 Aug 2018 12:39
 Operator : SY/MD
 Sample : J4599-02 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETOK4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

72	10.427	2962	2966	2967	rBV3	633	484	0.01%	0.002%
73	10.466	2975	2978	2980	rBV3	720	446	0.01%	0.002%
74	10.504	2988	2990	2993	rBV2	680	355	0.01%	0.002%
75	10.552	3001	3005	3006	rBV3	584	368	0.01%	0.002%
76	10.562	3006	3008	3011	rBV3	573	403	0.01%	0.002%
77	10.617	3019	3025	3026	rBV4	1265	1143	0.04%	0.006%
78	10.668	3038	3041	3046	rBV3	1025	777	0.02%	0.004%
79	10.739	3060	3063	3066	rBV5	618	381	0.01%	0.002%
80	10.803	3080	3083	3086	rVV2	743	588	0.02%	0.003%
81	10.903	3112	3114	3119	rBV3	674	546	0.02%	0.003%
82	10.935	3120	3124	3129	rVB4	985	875	0.03%	0.004%
83	11.173	3194	3198	3201	rVB4	592	446	0.01%	0.002%
84	11.302	3222	3238	3265	rBV	551507	995136	30.62%	4.890%
85	11.485	3292	3295	3298	rBV2	1020	683	0.02%	0.003%
86	11.565	3317	3320	3328	rVV6	1196	1545	0.05%	0.008%
87	11.597	3328	3330	3333	rVV3	742	519	0.02%	0.003%
88	11.630	3337	3340	3342	rBV	632	387	0.01%	0.002%
89	11.678	3342	3355	3379	rBV	567996	1027059	31.61%	5.047%
90	11.887	3416	3420	3422	rBV4	1133	976	0.03%	0.005%
91	12.006	3455	3457	3459	rBV2	673	362	0.01%	0.002%
92	12.141	3496	3499	3501	rBV3	841	651	0.02%	0.003%
93	12.539	3620	3623	3625	rBV4	753	518	0.02%	0.003%
94	12.642	3651	3655	3657	rBV2	769	741	0.02%	0.004%
95	12.810	3705	3707	3712	rVB4	872	608	0.02%	0.003%
96	12.903	3732	3736	3739	rBV3	876	912	0.03%	0.004%
97	13.359	3876	3878	3880	rBV3	984	406	0.01%	0.002%
98	13.449	3900	3906	3914	rVB3	10825	13798	0.42%	0.068%
99	13.739	3988	3996	4004	rBV2	12473	19506	0.60%	0.096%
100	14.427	4207	4210	4213	rBV4	1285	1190	0.04%	0.006%


Sum of corrected areas: 20348577

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082318\
Data File : VV007134.D
Acq On : 23 Aug 2018 12:39
Operator : SY/MD
Sample : J4599-02 20X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETOK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

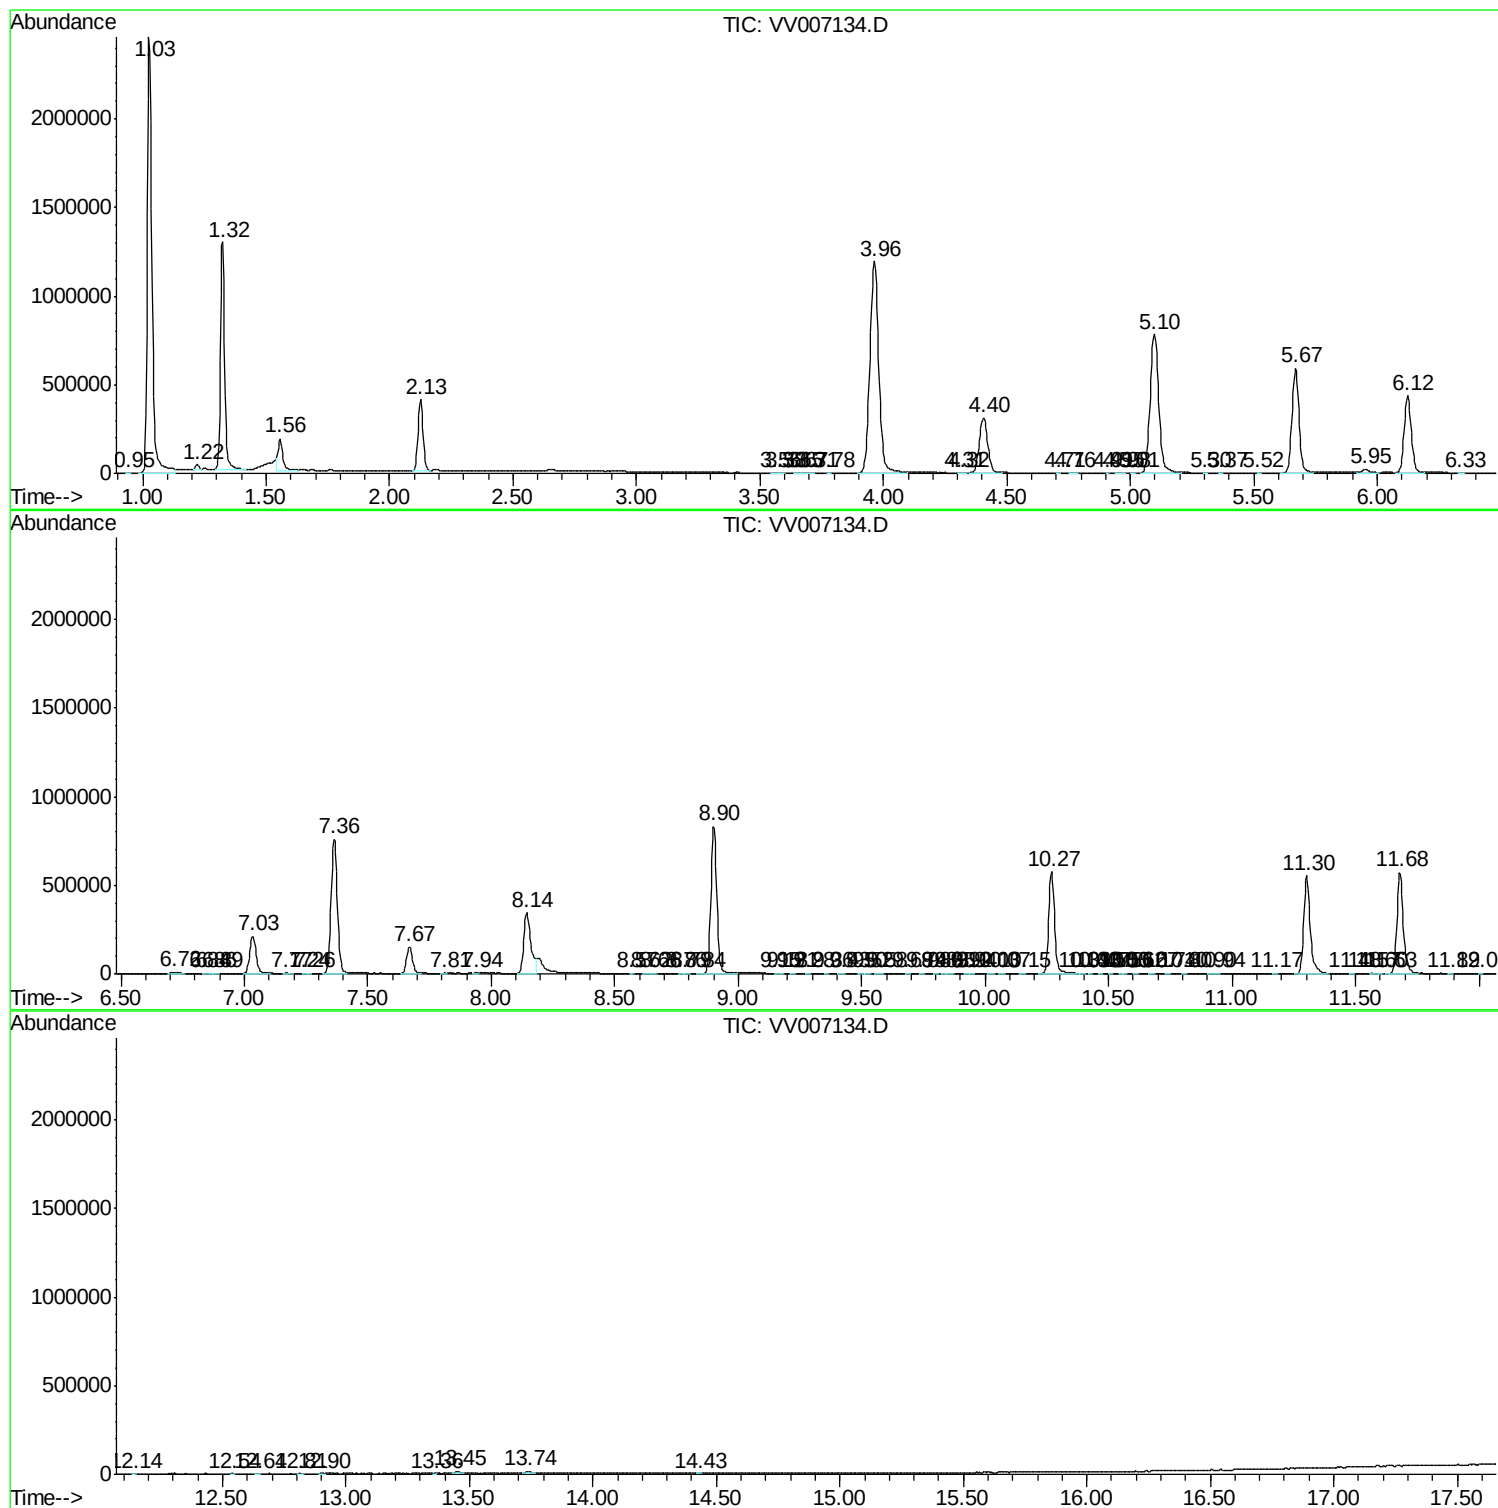

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082318\
Data File : VV007134.D
Acq On : 23 Aug 2018 12:39
Operator : SY/MD
Sample : J4599-02 20X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETOK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082318\
Data File : VV007134.D
Acq On : 23 Aug 2018 12:39
Operator : SY/MD
Sample : J4599-02 20X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETOK4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc