

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007135.D
 Acq On : 23 Aug 2018 13:05
 Operator : SY/MD
 Sample : J4599-03 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETOK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.029	26	43	82	rBV	2422437	3280347	98.90%	15.983%
2	1.221	98	103	108	rBV	27455	26296	0.79%	0.128%
3	1.324	126	135	172	rVB2	1398319	1654021	49.87%	8.059%
4	1.562	204	209	228	rVB	172370	214820	6.48%	1.047%
5	2.125	375	384	396	rBV	396054	555321	16.74%	2.706%
6	3.504	811	813	817	rBV2	481	315	0.01%	0.002%
7	3.575	829	835	841	rBV6	765	1194	0.04%	0.006%
8	3.713	869	878	885	rBV7	1402	2494	0.08%	0.012%
9	3.749	886	889	893	rBV4	629	364	0.01%	0.002%
10	3.768	893	895	896	rBV	564	314	0.01%	0.002%
11	3.829	911	914	917	rBV2	543	412	0.01%	0.002%
12	3.893	931	934	936	rBV4	781	494	0.01%	0.002%
13	3.964	936	956	997	rVV2	1335415	3316895	100.00%	16.161%
14	4.405	1076	1093	1116	rBV	307335	731046	22.04%	3.562%
15	4.556	1138	1140	1144	rVB2	849	514	0.02%	0.003%
16	4.720	1184	1191	1194	rBV7	839	826	0.02%	0.004%
17	4.810	1215	1219	1221	rVB2	637	448	0.01%	0.002%
18	4.823	1221	1223	1226	rBV3	678	378	0.01%	0.002%
19	4.877	1233	1240	1243	rBV4	763	753	0.02%	0.004%
20	4.906	1245	1249	1254	rVB5	824	765	0.02%	0.004%
21	4.945	1258	1261	1269	rVB4	662	842	0.03%	0.004%
22	5.099	1290	1309	1344	rBV2	780585	1863268	56.18%	9.078%
23	5.257	1355	1358	1360	rVB3	838	400	0.01%	0.002%
24	5.269	1360	1362	1365	rVB3	1038	682	0.02%	0.003%
25	5.298	1365	1371	1372	rBV3	847	909	0.03%	0.004%
26	5.376	1391	1395	1396	rBV3	1688	1091	0.03%	0.005%
27	5.440	1412	1415	1418	rBV4	796	555	0.02%	0.003%
28	5.517	1437	1439	1446	rVB6	1025	975	0.03%	0.005%
29	5.549	1446	1449	1452	rBV5	1034	748	0.02%	0.004%
30	5.581	1454	1459	1461	rBV5	1135	1053	0.03%	0.005%
31	5.668	1472	1486	1513	rBV	577288	1148896	34.64%	5.598%
32	5.948	1565	1573	1591	rVB3	17211	34575	1.04%	0.168%
33	6.125	1612	1628	1649	rBV	434807	865244	26.09%	4.216%
34	6.331	1690	1692	1696	rBV4	784	584	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007135.D
 Acq On : 23 Aug 2018 13:05
 Operator : SY/MD
 Sample : J4599-03 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETOK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

35	6.511	1744	1748	1750	rBV2	533	422	0.01%	0.002%
36	6.726	1805	1815	1825	rBV4	5184	10352	0.31%	0.050%
37	6.874	1858	1861	1865	rVB4	504	380	0.01%	0.002%
38	7.035	1898	1911	1929	rBV	205995	366660	11.05%	1.786%
39	7.157	1947	1949	1952	rBV4	755	429	0.01%	0.002%
40	7.366	1999	2014	2034	rBV	724721	1282865	38.68%	6.250%
41	7.668	2096	2108	2122	rBV	146656	244391	7.37%	1.191%
42	7.829	2155	2158	2160	rBV4	798	547	0.02%	0.003%
43	8.144	2244	2256	2267	rBV	359178	685039	20.65%	3.338%
44	8.539	2377	2379	2384	rVB4	942	565	0.02%	0.003%
45	8.649	2410	2413	2417	rBV4	778	595	0.02%	0.003%
46	8.707	2427	2431	2434	rBV3	1063	658	0.02%	0.003%
47	8.806	2456	2462	2464	rBV5	754	904	0.03%	0.004%
48	8.845	2471	2474	2478	rVB3	554	349	0.01%	0.002%
49	8.900	2478	2491	2513	rBV	811118	1333033	40.19%	6.495%
50	9.269	2603	2606	2607	rBV2	510	305	0.01%	0.001%
51	9.311	2614	2619	2620	rBV2	627	413	0.01%	0.002%
52	9.343	2626	2629	2630	rBV	742	329	0.01%	0.002%
53	9.478	2667	2671	2674	rVB2	560	364	0.01%	0.002%
54	9.501	2674	2678	2682	rBV5	1020	883	0.03%	0.004%
55	9.565	2694	2698	2701	rBV4	865	818	0.02%	0.004%
56	9.710	2740	2743	2748	rVB4	824	732	0.02%	0.004%
57	9.732	2748	2750	2753	rVB3	692	313	0.01%	0.002%
58	9.835	2779	2782	2786	rBV3	568	547	0.02%	0.003%
59	9.880	2792	2796	2799	rBV2	1270	1037	0.03%	0.005%
60	9.922	2807	2809	2813	rVB2	765	488	0.01%	0.002%
61	9.945	2813	2816	2817	rBV3	779	435	0.01%	0.002%
62	9.970	2821	2824	2827	rVB3	730	434	0.01%	0.002%
63	9.986	2827	2829	2833	rVB3	783	558	0.02%	0.003%
64	10.006	2833	2835	2836	rBV	666	307	0.01%	0.001%
65	10.083	2855	2859	2863	rBV3	835	847	0.03%	0.004%
66	10.102	2863	2865	2869	rVB4	516	317	0.01%	0.002%
67	10.134	2869	2875	2878	rBV7	941	809	0.02%	0.004%
68	10.157	2880	2882	2887	rVV3	324	308	0.01%	0.002%
69	10.208	2893	2898	2901	rBV3	688	616	0.02%	0.003%
70	10.269	2904	2917	2938	rBV	577664	922951	27.83%	4.497%
71	10.449	2971	2973	2975	rVB2	919	374	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007135.D
 Acq On : 23 Aug 2018 13:05
 Operator : SY/MD
 Sample : J4599-03 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETOK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Title : VOC Analysis

72	10.469	2976	2979	2982	rVB3	823	512	0.02%	0.002%
73	10.507	2988	2991	2993	rBV3	622	422	0.01%	0.002%
74	10.552	3003	3005	3010	rVB2	702	546	0.02%	0.003%
75	10.613	3021	3024	3028	rBV3	612	577	0.02%	0.003%
76	10.655	3035	3037	3040	rVB	764	375	0.01%	0.002%
77	10.858	3098	3100	3103	rVB3	647	341	0.01%	0.002%
78	10.906	3112	3115	3118	rBV2	756	504	0.02%	0.002%
79	10.961	3128	3132	3134	rBV2	633	521	0.02%	0.003%
80	10.993	3139	3142	3144	rBV2	771	467	0.01%	0.002%
81	11.063	3160	3164	3165	rBV3	916	701	0.02%	0.003%
82	11.150	3188	3191	3193	rVB	881	515	0.02%	0.003%
83	11.166	3193	3196	3197	rBV2	788	403	0.01%	0.002%
84	11.301	3225	3238	3267	rBV	556318	942957	28.43%	4.594%
85	11.581	3321	3325	3327	rBV2	1009	842	0.03%	0.004%
86	11.678	3343	3355	3379	rVV	579948	988857	29.81%	4.818%
87	11.838	3403	3405	3411	rVB5	755	604	0.02%	0.003%
88	11.948	3437	3439	3443	rVB3	1024	698	0.02%	0.003%
89	12.211	3519	3521	3525	rVB5	895	589	0.02%	0.003%
90	12.234	3525	3528	3530	rBV2	542	433	0.01%	0.002%
91	12.250	3531	3533	3536	rVB3	786	418	0.01%	0.002%
92	12.588	3635	3638	3641	rVB2	1231	821	0.02%	0.004%
93	12.922	3739	3742	3745	rBV2	1027	915	0.03%	0.004%
94	12.989	3758	3763	3765	rBV4	874	885	0.03%	0.004%
95	13.269	3848	3850	3853	rVB3	1437	768	0.02%	0.004%
96	13.385	3884	3886	3888	rBV3	957	602	0.02%	0.003%
97	13.742	3991	3997	4004	rBV7	5438	6817	0.21%	0.033%
98	13.813	4017	4019	4023	rVB4	1240	821	0.02%	0.004%
99	13.867	4033	4036	4037	rBV2	1111	689	0.02%	0.003%
100	14.481	4225	4227	4235	rVB5	1662	1406	0.04%	0.007%


Sum of corrected areas: 20524219

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082318\
Data File : VV007135.D
Acq On : 23 Aug 2018 13:05
Operator : SY/MD
Sample : J4599-03 20X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETOK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

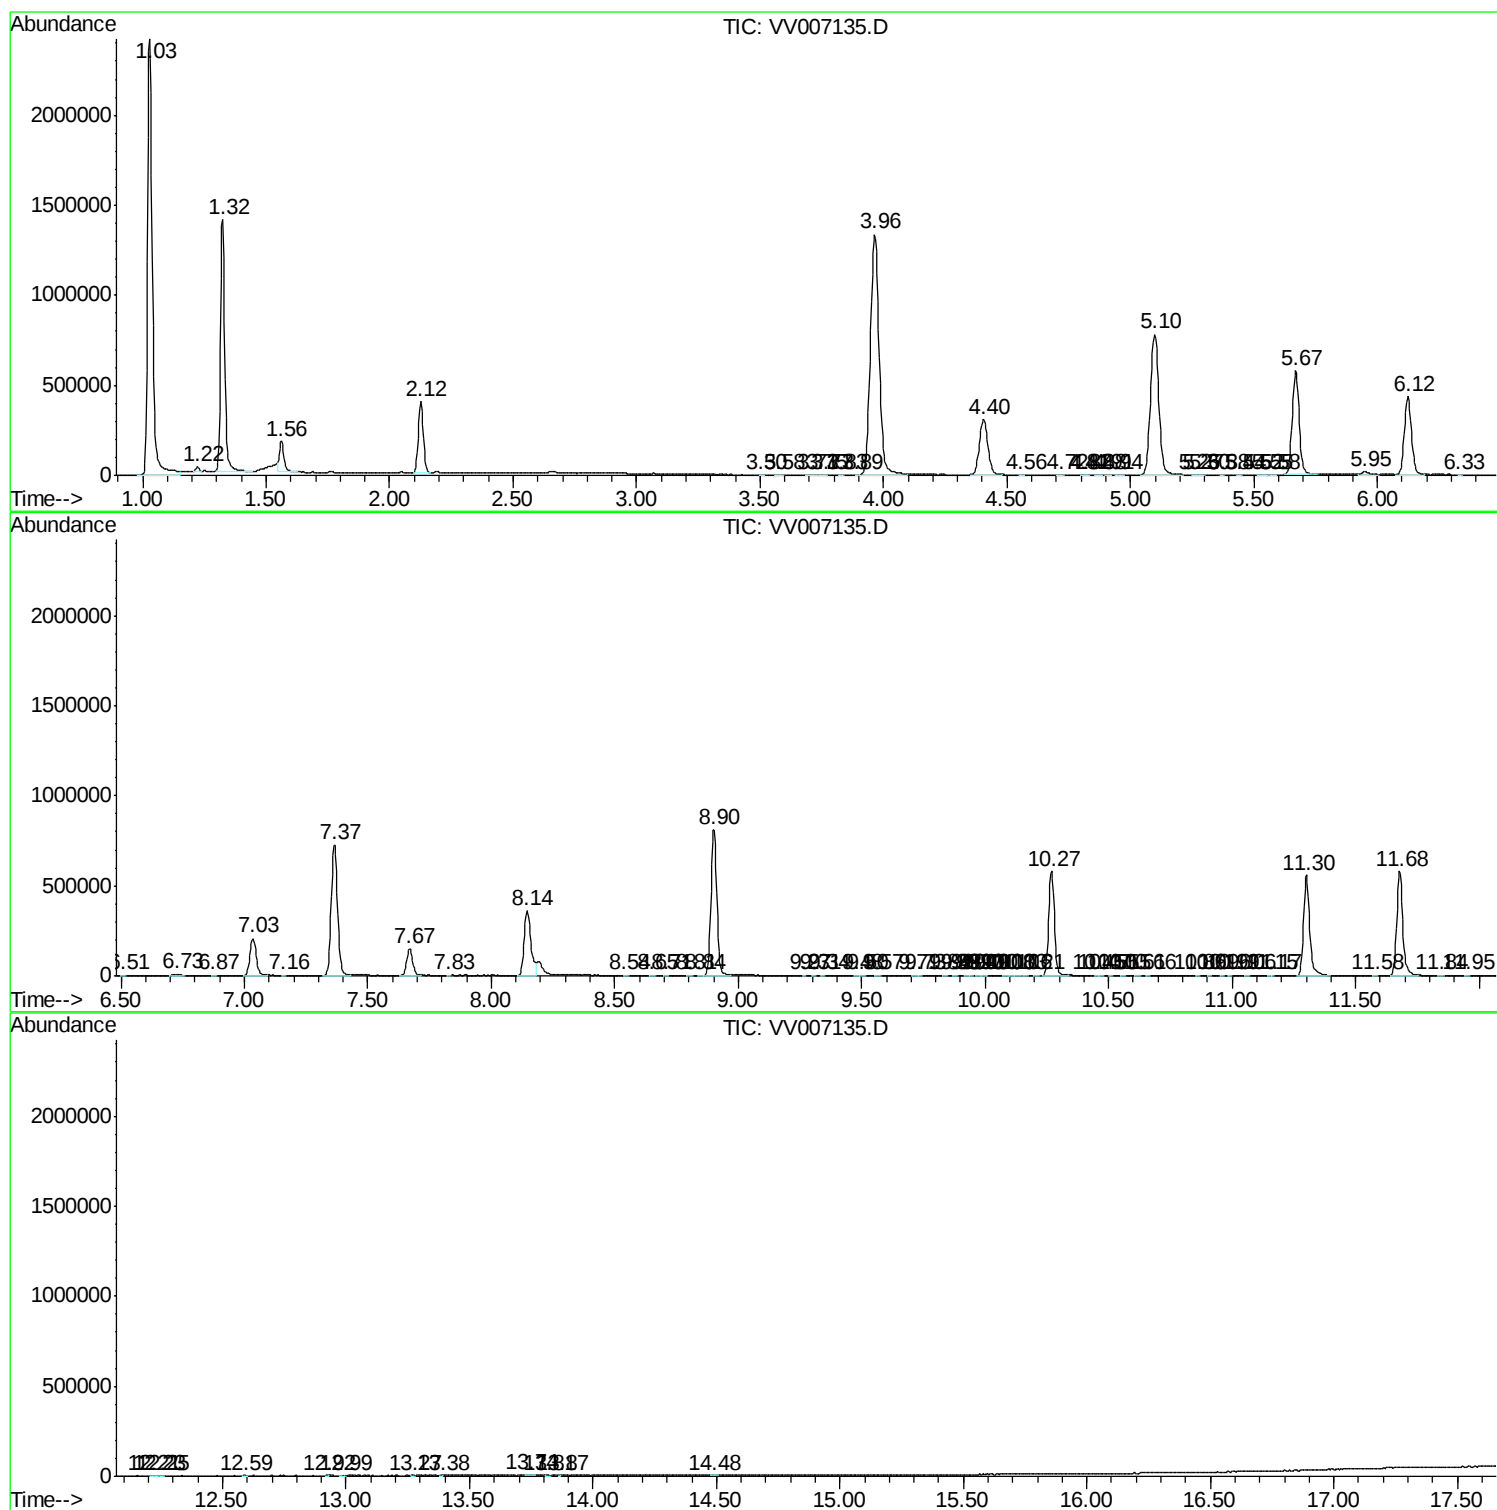

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082318\
Data File : VV007135.D
Acq On : 23 Aug 2018 13:05
Operator : SY/MD
Sample : J4599-03 20X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETOK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082318\
Data File : VV007135.D
Acq On : 23 Aug 2018 13:05
Operator : SY/MD
Sample : J4599-03 20X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETOK5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc