


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
Data File : VV007128.D
Acq On : 23 Aug 2018 08:58
Operator : SY/MD
Sample : BFB63
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Title : VOC Analysis
Last Update : Fri Aug 24 02:07:07 2018

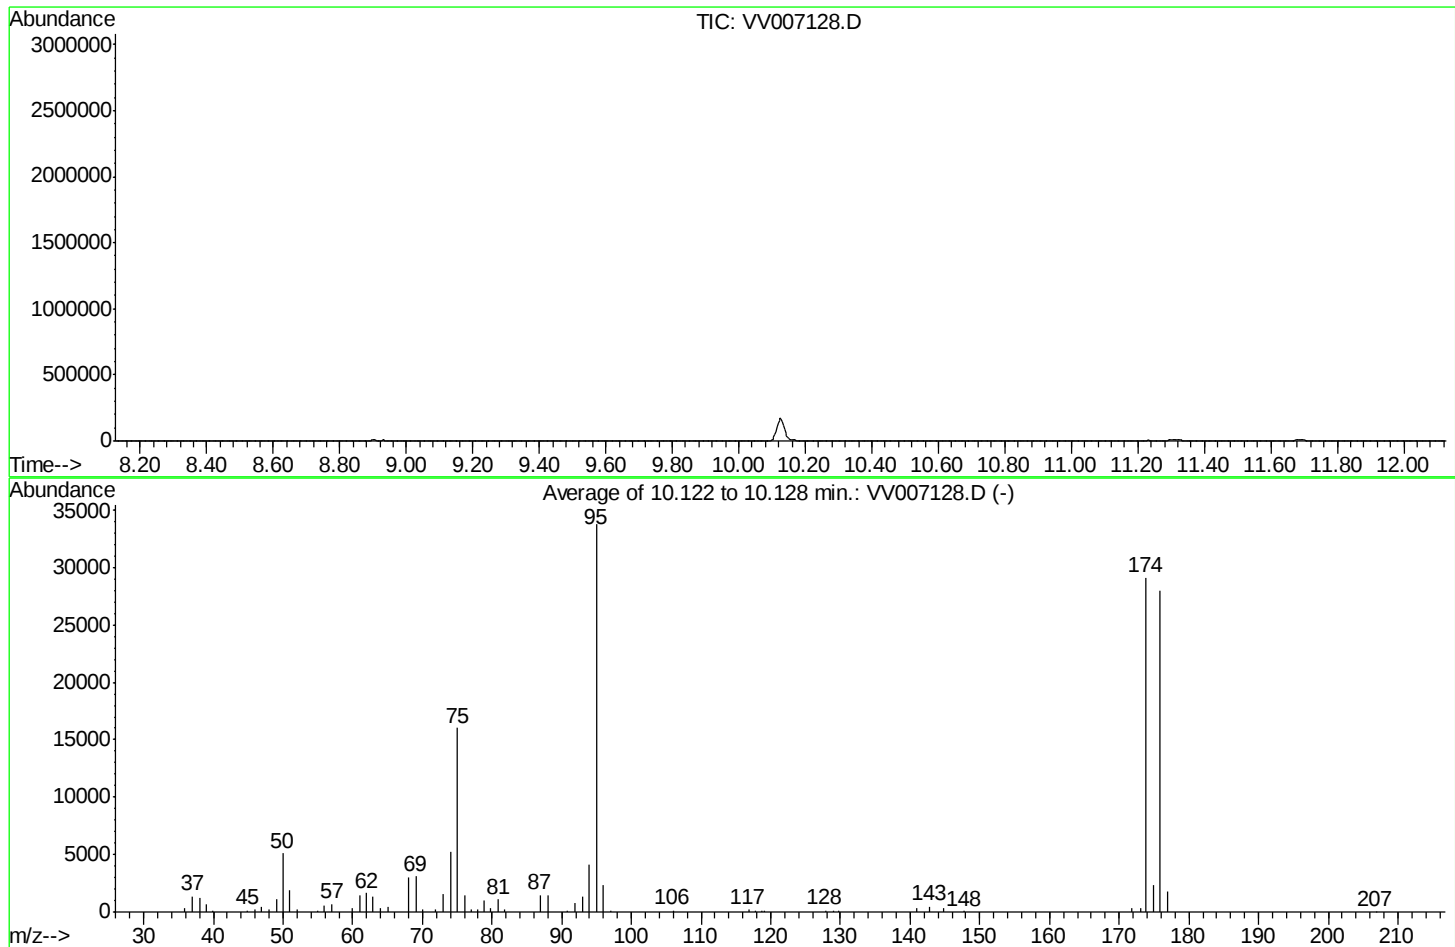

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	5118	PASS
75	95	30	80	47.4	16014	PASS
95	95	100	100	100.0	33757	PASS
96	95	5	9	7.0	2377	PASS
173	174	0.00	2	1.0	301	PASS
174	95	50	120	86.3	29136	PASS
175	174	5	9	8.2	2376	PASS
176	174	95	101	96.0	27968	PASS
177	176	5	9	6.5	1804	PASS

Scan 2860 (10.086 min): VV007128.D
BFB63

m/z	Abundance
39.90	343.0
43.90	1166.0
45.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.10	294.0
37.00	1384.0
38.00	1243.0
38.90	595.0
39.90	450.0
43.90	1125.0
44.90	247.0
46.00	189.0
46.90	435.0
47.90	220.0
49.00	1112.0
50.00	4913.0
51.00	1839.0
52.00	151.0
54.90	116.0
56.10	489.0
57.00	759.0
59.90	323.0
61.00	1495.0
62.00	1546.0
63.00	1463.0
63.90	341.0
65.00	502.0
68.00	2924.0
69.00	3022.0
70.00	247.0
72.00	248.0
73.00	1476.0
74.00	5014.0
75.00	15604.0
76.00	1485.0
77.10	227.0
77.90	279.0
78.90	1014.0
79.90	273.0
80.90	1073.0
81.80	188.0
86.90	1476.0
87.90	1502.0
91.80	762.0
93.00	1148.0
94.00	4079.0
95.00	32456.0
96.00	2316.0
106.00	178.0
116.90	191.0
117.80	117.0
118.70	179.0
127.80	175.0
129.00	117.0
129.70	115.0
140.90	281.0
142.80	442.0
144.80	325.0
171.70	254.0
173.90	26720.0
174.90	2192.0
175.90	26896.0
176.90	1571.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.90	353.0
37.00	1408.0
38.00	1260.0
38.90	661.0
39.90	489.0
43.90	1126.0
44.90	237.0
46.00	205.0
46.90	466.0
47.90	260.0
49.00	1113.0
50.00	5218.0
51.00	1974.0
51.90	188.0
54.90	107.0
55.90	566.0
57.00	744.0
59.90	302.0
61.00	1469.0
62.00	1718.0
63.00	1462.0
63.90	310.0
65.00	462.0
68.00	3041.0
69.00	3200.0
70.00	257.0
72.00	209.0
73.00	1616.0
74.00	5394.0
75.00	16560.0
76.00	1541.0
77.00	244.0
77.90	274.0
78.90	1005.0
79.80	313.0
80.90	1111.0
81.80	255.0
86.90	1527.0
88.00	1579.0
90.70	107.0
91.80	758.0
93.00	1311.0
94.00	4305.0
95.00	34840.0
96.00	2478.0
97.10	105.0
106.00	146.0
116.80	212.0
117.80	136.0
118.80	175.0
127.80	180.0
129.00	146.0
129.80	116.0
141.00	308.0
142.80	475.0
144.80	287.0
147.80	139.0
171.80	296.0
173.10	429.0
173.90	30064.0
174.90	2485.0
175.90	28912.0
176.90	1798.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.90	370.0
37.00	1296.0
38.00	1195.0
39.00	645.0
39.90	465.0
43.90	1163.0
44.90	259.0
46.00	171.0
47.00	532.0
47.90	228.0
49.00	1033.0
50.00	5224.0
51.00	1857.0
51.90	226.0
54.90	105.0
55.90	590.0
57.00	637.0
59.80	277.0
60.90	1491.0
62.00	1706.0
62.90	1244.0
63.90	265.0
65.00	381.0
68.00	2976.0
69.10	3099.0
70.00	206.0
71.90	173.0
73.00	1549.0
74.00	5239.0
75.00	15878.0
76.00	1494.0
77.00	298.0
78.00	214.0
78.90	947.0
79.80	331.0
80.90	1066.0
81.90	282.0
86.90	1499.0
87.90	1311.0
90.80	114.0
91.90	729.0
93.00	1469.0
94.00	4029.0
95.00	33976.0
96.00	2338.0
97.10	138.0
106.00	106.0
116.80	224.0
117.80	150.0
119.00	181.0
127.80	136.0
128.90	122.0
129.90	113.0
141.00	281.0
142.90	517.0
144.80	262.0
147.80	153.0
171.80	404.0
173.00	476.0
173.90	30624.0
174.90	2452.0
175.90	28096.0
177.00	2045.0
206.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63