

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082319\
 Data File : VV012369.D
 Acq On : 23 Aug 2019 17:43
 Operator : SY/MD
 Sample : K4481-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COXM0

Quant Time: Aug 26 08:15:44 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 26 07:59:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	269412	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	260843	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	103990	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65722	4.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.60%
7) Chloroethane-d5	1.58	69	49172	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.00%
11) 1,1-Dichloroethene-d2	2.13	63	88675	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	3.97	46	185376	51.09	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.18%
24) Chloroform-d	4.40	84	144222	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.08	65	73696	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.10	84	301326	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.12	67	92886	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.36	98	250592	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
43) trans-1,3-Dichloropropene-	7.67	79	30457	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.14	63	96767	42.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.52%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	56752	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	86734	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Ovalue
13) Acetone	2.23	43	9001	5.733 ug/L	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082319\
Data File : VV012369.D
Acq On : 23 Aug 2019 17:43
Operator : SY/MD
Sample : K4481-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XM0

Quant Time: Aug 26 08:15:44 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 26 07:59:52 2019
Response via : Initial Calibration

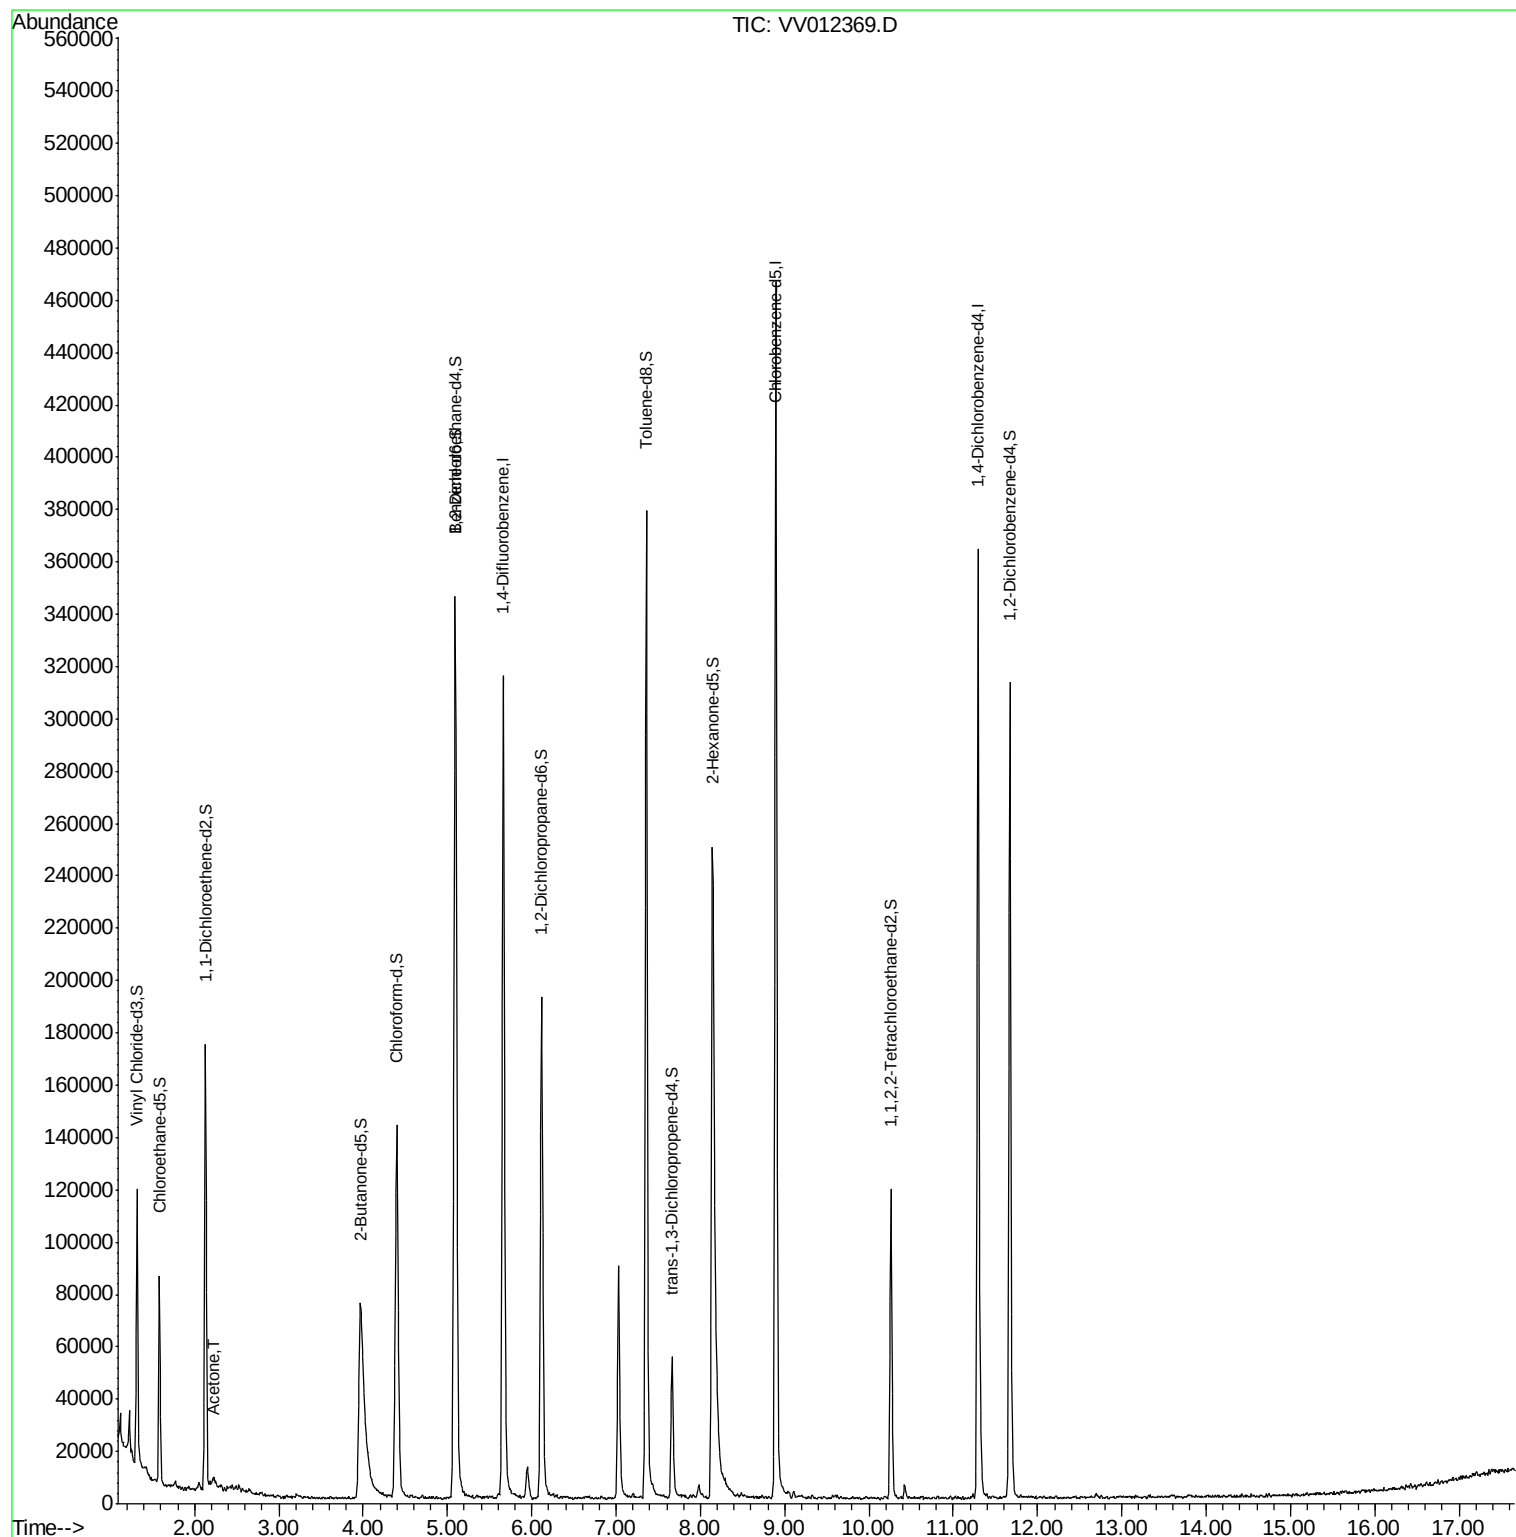

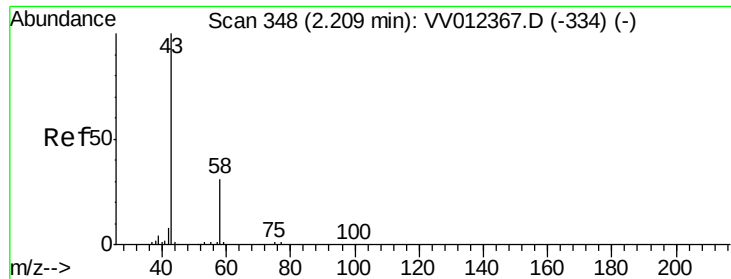

#13

Acetone

Concen: 5.733 ug/L

RT: 2.23 min Scan# 354

Delta R.T. 0.02 min

Lab File: VV012369.D

Acq: 23 Aug 2019 17:43


Instrument :
MSVOA_V
ClientSampleId :
C0XM0

Tot Ion: 43 Resp: 9001

Ion Ratio Lower Upper

43 100

58 8.1 0.0 62.8

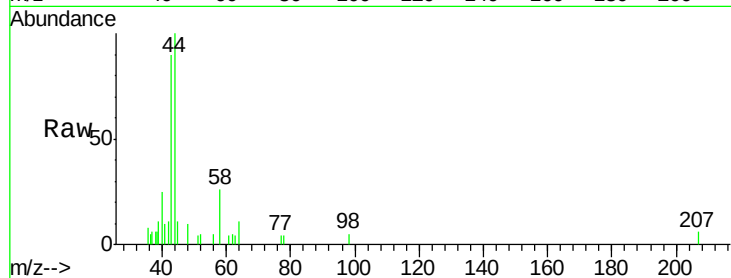

Abundance Ion 43.05 (42.75 to 43.75): VV0
Ion 58.05 (57.75 to 58.75): VV0

