


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082319\
Data File : VV012358.D
Acq On : 23 Aug 2019 11:41
Operator : SY/MD
Sample : BFB52
Misc : 5mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB52

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 27 02:19:39 2019

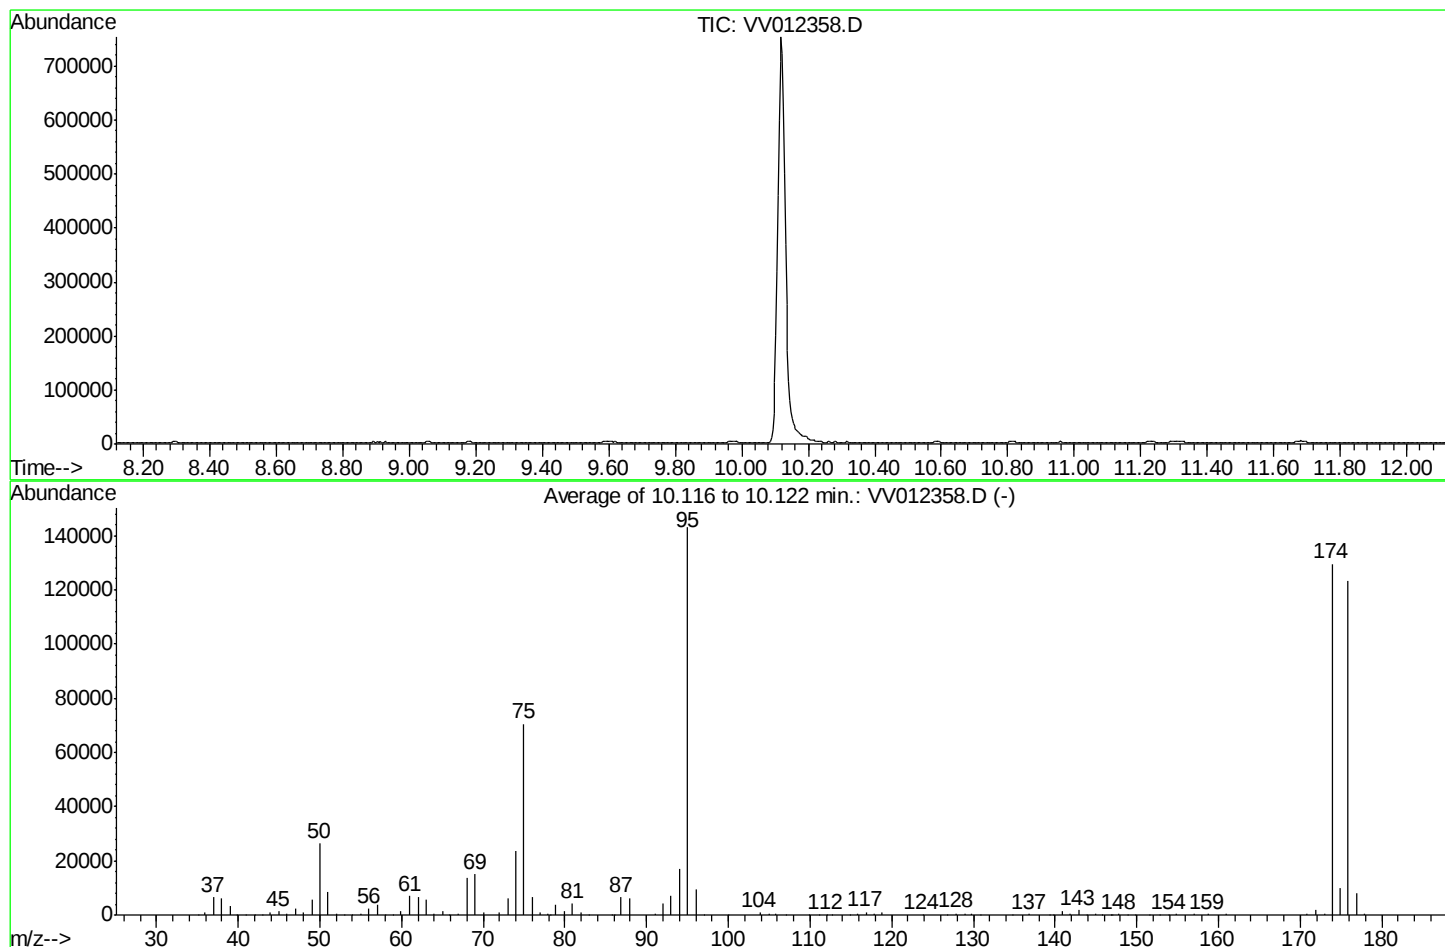

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	26402	PASS
75	95	30	80	49.4	70592	PASS
95	95	100	100	100.0	143018	PASS
96	95	5	9	6.7	9541	PASS
173	174	0.00	2	0.4	500	PASS
174	95	50	120	90.5	129477	PASS
175	174	5	9	7.8	10137	PASS
176	174	95	101	95.1	123165	PASS
177	176	5	9	6.4	7855	PASS

m/z	Abundance
35.10	120.0
36.00	1285.0
37.00	6560.0
38.00	6059.0
39.00	3160.0
39.90	1107.0
40.90	138.0
42.00	123.0
42.90	155.0
44.00	1608.0
45.00	1117.0
46.00	346.0
47.00	2318.0
48.00	843.0
49.00	5637.0
50.00	26072.0
51.00	8385.0
52.00	403.0
53.00	108.0
53.80	138.0
55.00	467.0
56.00	2307.0
57.00	3813.0
58.10	198.0
58.90	105.0
60.00	1233.0
61.00	6892.0
62.00	6440.0
63.00	5646.0
64.00	742.0
65.00	1399.0
65.90	282.0
67.10	372.0
68.00	13628.0
69.00	14767.0
70.00	1197.0
71.90	881.0
73.00	6142.0
74.00	23408.0
75.00	69184.0
76.00	6535.0
77.00	763.0
77.90	729.0
78.90	3951.0
79.90	1378.0
80.90	4084.0
81.90	884.0
82.90	197.0
85.70	154.0
86.10	252.0
86.90	6155.0
87.90	6084.0
91.10	569.0
92.00	4071.0
93.00	6635.0
94.00	16251.0
95.00	138496.0
96.00	9892.0
96.90	279.0
103.80	694.0
104.90	274.0
105.80	700.0
109.80	136.0
111.10	119.0
112.00	150.0
112.70	126.0
114.80	169.0
115.80	534.0
116.90	1052.0
117.90	541.0
118.90	967.0
123.80	115.0
126.90	109.0
127.90	601.0
129.00	343.0
129.80	569.0
130.90	259.0
134.80	212.0
136.90	274.0
139.20	108.0
139.90	135.0
140.80	1310.0
141.90	261.0
142.90	1666.0
143.90	169.0
144.90	484.0
145.70	280.0
147.10	144.0
147.80	332.0
148.80	133.0
149.90	174.0
153.90	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

154.80	269.0
157.00	296.0
158.70	257.0
161.00	218.0
170.80	272.0
171.90	1647.0
173.00	1501.0
173.90	123184.0
174.90	9523.0
175.90	118400.0
176.90	7733.0
177.90	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
36.00	1241.0
37.00	6685.0
38.00	6296.0
39.00	3300.0
39.90	1113.0
40.90	118.0
42.00	127.0
42.90	179.0
44.00	1591.0
44.90	1241.0
46.00	344.0
47.00	2534.0
48.00	945.0
49.00	5824.0
50.00	27456.0
51.00	8733.0
52.00	414.0
53.00	134.0
53.90	138.0
54.90	445.0
56.00	2293.0
57.00	4020.0
58.00	189.0
59.00	125.0
59.90	1346.0
61.00	7096.0
62.00	6659.0
63.00	5891.0
64.00	726.0
65.00	1466.0
65.90	214.0
66.90	397.0
68.00	14233.0
69.00	15770.0
70.00	1179.0
71.90	976.0
73.00	6398.0
74.00	24312.0
75.00	73152.0
76.00	6616.0
77.00	779.0
77.90	765.0
78.90	4160.0
79.90	1420.0
80.90	4267.0
81.90	873.0
82.90	163.0
85.70	198.0
86.10	200.0
86.90	6662.0
87.90	6436.0
91.10	617.0
92.00	4283.0
93.00	7201.0
94.00	17536.0
95.00	148160.0
96.00	9783.0
97.00	247.0
103.80	831.0
104.90	288.0
105.80	687.0
109.80	130.0
111.10	135.0
112.00	142.0
112.70	162.0
114.80	209.0
115.90	610.0
116.90	1020.0
117.90	622.0
118.80	1079.0
123.70	144.0
126.80	135.0
127.90	590.0
129.00	376.0
129.80	629.0
130.90	230.0
134.80	239.0
136.80	278.0
139.30	119.0
139.80	145.0
140.80	1476.0
141.80	291.0
142.90	1817.0
143.80	181.0
144.90	485.0
145.70	262.0
147.00	116.0
147.80	358.0
148.80	150.0
149.80	191.0
152.80	124.0
153.90	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

154.80	264.0
157.00	271.0
158.70	296.0
161.00	299.0
170.70	280.0
171.90	1743.0
173.90	134208.0
174.90	10584.0
175.90	127528.0
176.90	8108.0
177.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
36.00	1194.0
37.00	6032.0
38.00	5880.0
39.00	3086.0
39.90	1131.0
42.00	118.0
42.90	199.0
44.00	1589.0
44.90	1289.0
46.00	286.0
47.00	2430.0
48.00	933.0
49.00	5439.0
50.00	25680.0
51.00	8212.0
52.10	371.0
53.00	159.0
54.00	109.0
54.90	379.0
56.00	1945.0
57.00	3888.0
57.90	174.0
59.00	124.0
59.90	1227.0
61.00	6635.0
62.00	6471.0
63.00	5558.0
64.00	665.0
65.00	1394.0
65.90	162.0
66.90	399.0
68.00	13665.0
69.00	14949.0
70.00	1066.0
72.00	906.0
73.00	6033.0
74.00	22608.0
75.00	69440.0
76.00	6096.0
77.00	670.0
77.80	686.0
78.20	573.0
78.90	3977.0
79.90	1338.0
80.90	4092.0
81.90	824.0
82.80	117.0
85.70	219.0
86.90	6510.0
87.90	6105.0
91.00	562.0
91.90	4061.0
93.00	6950.0
94.00	17152.0
95.00	142400.0
96.00	8950.0
97.00	212.0
100.00	115.0
103.90	848.0
105.00	292.0
105.80	626.0
107.00	103.0
111.00	105.0
112.00	141.0
112.80	165.0
114.90	217.0
115.90	584.0
116.90	861.0
117.90	633.0
118.80	1102.0
123.70	151.0
126.80	130.0
127.90	556.0
128.90	348.0
129.80	548.0
130.90	199.0
134.80	247.0
136.80	238.0
139.80	142.0
140.90	1496.0
141.80	228.0
142.90	1741.0
143.80	193.0
144.90	383.0
145.80	221.0
146.80	107.0
147.90	375.0
148.90	147.0
149.80	173.0
151.60	116.0
152.80	137.0
153.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

154.80	262.0
156.90	257.0
158.80	295.0
160.90	301.0
170.80	239.0
171.90	1769.0
173.90	131040.0
174.90	10306.0
175.90	123568.0
176.90	7724.0
177.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

Scan 2794 (10.074 min): VV012358.D
BFB52

m/z	Abundance
35.80	134.0
40.00	949.0
43.90	827.0
65.90	102.0
69.10	131.0
118.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52