


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082321\
 Data File : VV021925.D
 Acq On : 23 Aug 2021 08:52
 Operator : SY/MD
 Sample : BFB220
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB220

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 24 02:24:25 2021

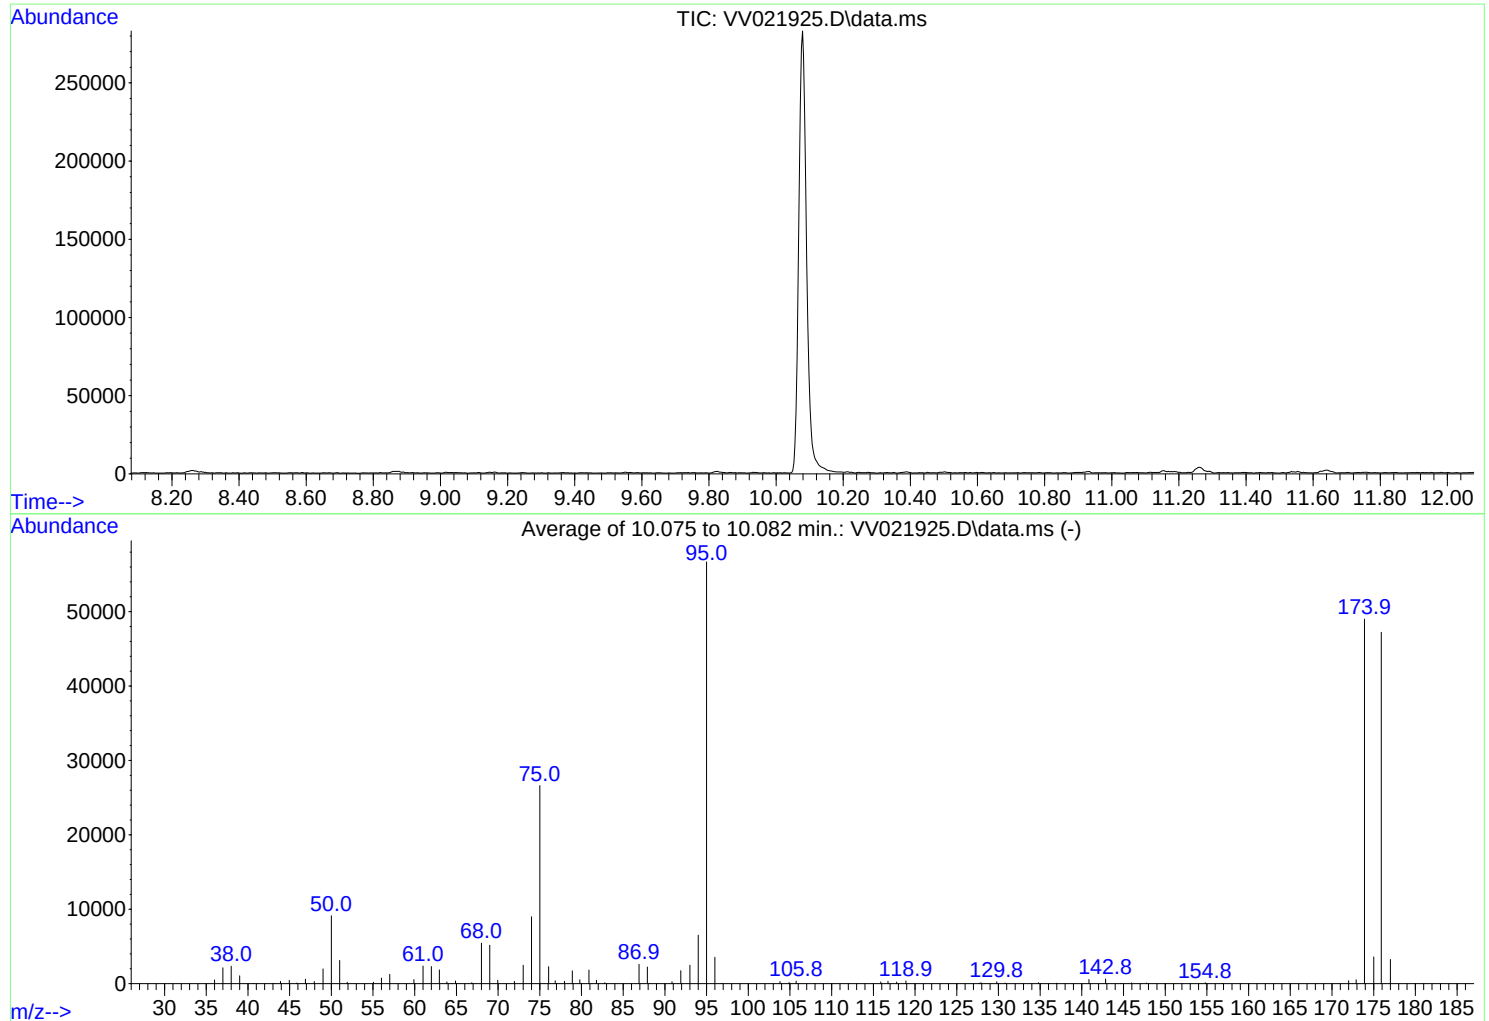

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	9113	PASS
75	95	30	80	46.9	26621	PASS
95	95	100	100	100.0	56701	PASS
96	95	5	9	6.3	3550	PASS
173	174	0.00	2	1.0	514	PASS
174	95	50	120	86.4	49005	PASS
175	174	5	9	7.3	3590	PASS
176	174	95	105	96.4	47245	PASS
177	176	5	10	6.9	3239	PASS

m/z	Abundance
39.90	216.0
43.90	351.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	512.0
37.00	2063.0
38.00	2361.0
39.00	1084.0
40.00	206.0
44.00	672.0
45.00	483.0
46.90	593.0
47.90	335.0
49.00	2100.0
50.00	9202.0
51.00	3239.0
51.90	191.0
55.10	180.0
56.00	775.0
57.00	1277.0
59.90	488.0
61.00	2331.0
62.00	2291.0
63.00	1824.0
63.90	234.0
64.90	349.0
66.90	132.0
68.00	5476.0
69.00	5240.0
69.90	448.0
71.90	269.0
73.00	2501.0
74.00	9122.0
75.00	26824.0
76.00	2289.0
76.80	423.0
78.00	379.0
78.90	1693.0
79.80	470.0
80.90	1842.0
81.80	453.0
82.80	138.0
86.90	2606.0
87.90	2313.0
90.80	283.0
91.90	1690.0
93.00	2455.0
94.00	6765.0
95.00	56832.0
96.00	3534.0
96.80	102.0
103.80	262.0
104.90	155.0
105.70	357.0
115.90	223.0
116.70	328.0
117.80	240.0
118.90	336.0
127.70	202.0
129.70	272.0
130.80	130.0
134.80	144.0
140.80	524.0
142.80	626.0
146.00	119.0
154.80	128.0
156.80	107.0
171.90	396.0
172.90	548.0
173.90	47368.0
175.00	3612.0
175.90	46200.0
177.00	3148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	522.0
37.00	2163.0
38.00	2458.0
39.00	1126.0
39.90	163.0
43.90	666.0
45.00	458.0
45.80	115.0
46.90	602.0
47.90	295.0
49.00	2020.0
50.00	9461.0
51.00	3274.0
51.90	213.0
55.00	189.0
56.00	750.0
57.00	1278.0
59.90	578.0
61.00	2380.0
62.00	2380.0
63.00	1924.0
63.90	252.0
64.90	381.0
66.80	120.0
68.00	5632.0
69.00	5329.0
70.00	459.0
71.90	300.0
73.00	2557.0
74.00	9329.0
75.00	27416.0
76.00	2386.0
76.90	397.0
78.00	340.0
78.90	1785.0
79.80	535.0
80.90	1922.0
81.80	442.0
82.80	150.0
86.90	2664.0
87.90	2276.0
90.80	256.0
91.90	1809.0
93.00	2552.0
94.00	6675.0
95.00	58568.0
96.00	3621.0
103.80	294.0
104.90	158.0
105.70	367.0
115.90	270.0
116.70	340.0
117.80	227.0
118.90	384.0
127.90	207.0
129.80	266.0
130.80	101.0
134.80	140.0
137.00	107.0
140.80	579.0
142.90	642.0
145.90	119.0
147.70	117.0
154.80	130.0
172.00	387.0
172.90	530.0
173.90	50792.0
175.00	3741.0
175.90	48704.0
177.00	3384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	471.0
37.00	2147.0
38.00	2197.0
39.00	968.0
39.90	143.0
40.70	129.0
43.10	112.0
43.90	651.0
44.90	417.0
45.90	112.0
46.90	610.0
48.00	244.0
49.00	1827.0
50.00	8676.0
51.00	2866.0
51.90	194.0
55.00	183.0
56.00	711.0
57.00	1200.0
59.90	553.0
61.00	2379.0
62.00	2205.0
62.90	1804.0
63.80	232.0
64.90	370.0
66.80	122.0
68.00	5221.0
69.00	4947.0
70.00	472.0
72.00	335.0
73.00	2340.0
74.00	8537.0
75.00	25624.0
76.10	2177.0
76.90	324.0
77.90	254.0
78.90	1657.0
79.80	574.0
80.90	1739.0
81.80	436.0
82.80	115.0
86.90	2549.0
87.90	2111.0
90.90	224.0
91.90	1748.0
93.00	2426.0
94.00	6126.0
95.00	54704.0
96.00	3496.0
103.80	280.0
104.90	132.0
105.80	339.0
115.90	243.0
116.80	322.0
117.80	200.0
118.90	371.0
127.90	215.0
129.90	259.0
134.80	138.0
137.00	111.0
140.90	581.0
142.90	609.0
144.70	106.0
145.90	109.0
147.80	143.0
154.80	135.0
172.10	387.0
172.90	463.0
173.90	48856.0
175.00	3416.0
175.90	46832.0
177.00	3184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220