




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
 Data File : VV027486.D
 Acq On : 23 Aug 2022 15:39
 Operator : SY/MD
 Sample : N4252-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 24 02:13:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 24 02:11:24 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/24/2022
 Supervised By :Mahesh Dadoda 08/25/2022

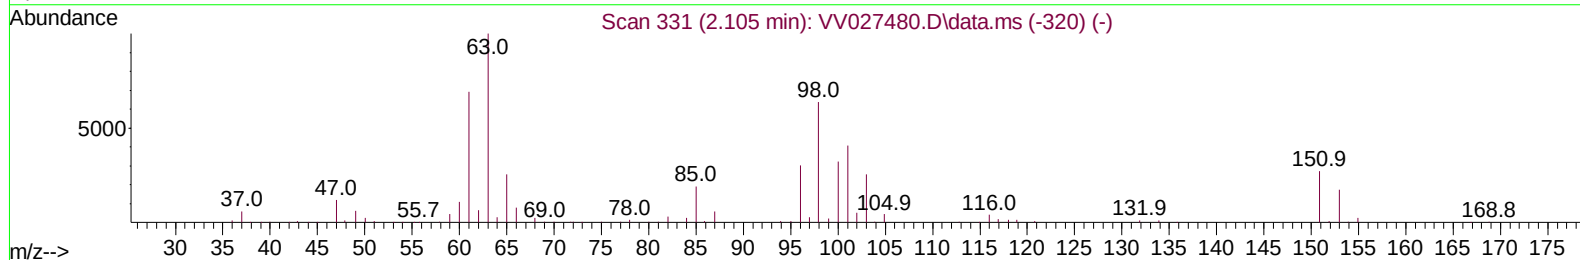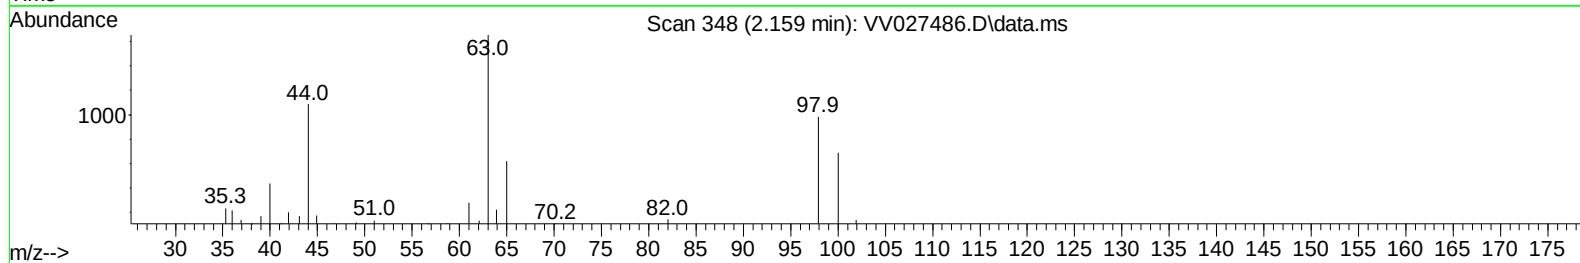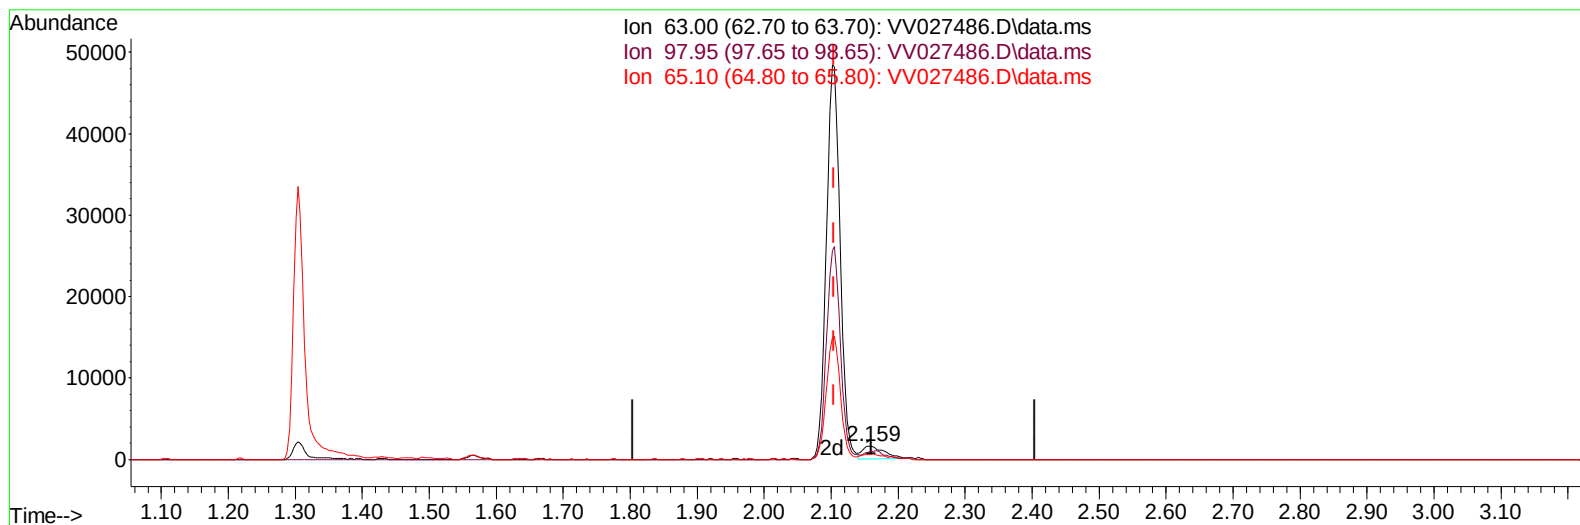

TIC: VV027486.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.159min (+ 0.055) 0.17 ug/L

response 3554

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	53.21
65.10	22.40	24.28
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
 Data File : VV027486.D
 Acq On : 23 Aug 2022 15:39
 Operator : SY/MD
 Sample : N4252-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/24/2022
 Supervised By :Mahesh Dadoda 08/25/2022

Quant Time: Aug 24 02:13:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 24 02:11:24 2022
 Response via : Initial Calibration

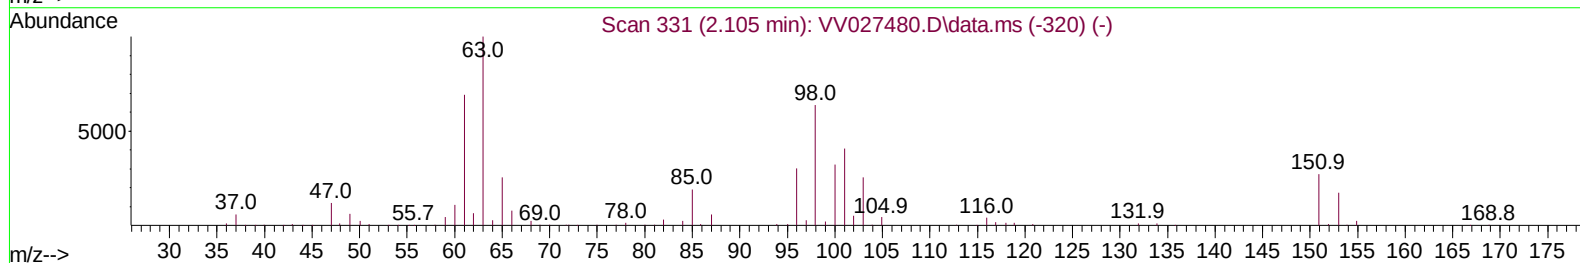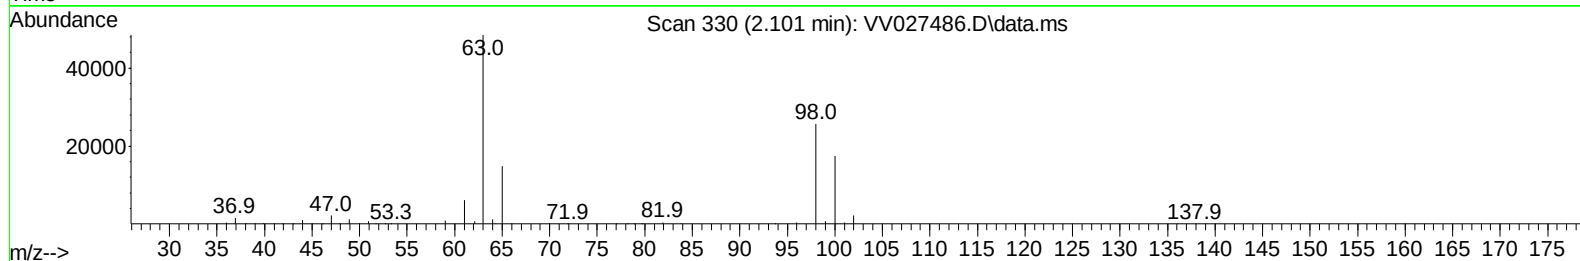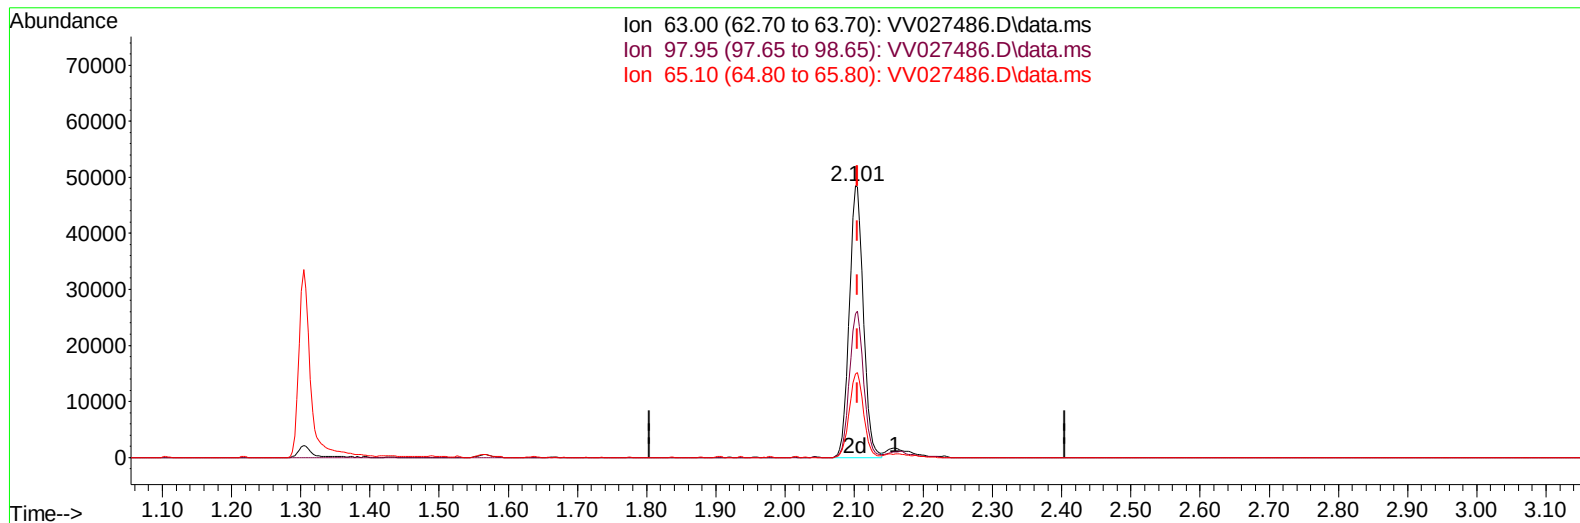

TIC: VV027486.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 3.34 ug/L m

response 69267

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	2.73#
65.10	22.40	1.25#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
 Data File : VV027486.D
 Acq On : 23 Aug 2022 15:39
 Operator : SY/MD
 Sample : N4252-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 24 02:13:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 24 02:11:24 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/24/2022
 Supervised By :Mahesh Dadoda 08/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.609	114		124808	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		127105	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		56086	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		40102	4.515	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%	
7) Chloroethane-d5	1.564	69		35757	5.500	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.000%	
11) 1,1-Dichloroethene-d2	2.101	63		69267m	3.344	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.800%	
20) 2-Butanone-d5	3.889	46		33019	29.870	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	59.740%	
24) Chloroform-d	4.339	84		74945	4.220	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%	
26) 1,2-Dichloroethane-d4	5.027	65		34607	4.504	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%	
32) Benzene-d6	5.043	84		137638	3.909	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%	
36) 1,2-Dichloropropane-d6	6.063	67		42024	4.106	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.200%	
41) Toluene-d8	7.313	98		112542	3.540	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.800%	
43) trans-1,3-Dichloroprop...	7.622	79		13396	3.822	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%	
46) 2-Hexanone-d5	8.088	63		40256	34.894	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.780%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		30089	4.616	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		37225	4.477	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.600%	
Target Compounds							
16) Methylene chloride	2.503	84		4389	0.308	ug/L	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
Data File : VV027486.D
Acq On : 23 Aug 2022 15:39
Operator : SY/MD
Sample : N4252-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 24 02:13:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 24 02:11:24 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/24/2022
Supervised By :Mahesh Dadoda 08/25/2022

