

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
 Data File : VV027482.D
 Acq On : 23 Aug 2022 12:26
 Operator : SY/MD
 Sample : N4253-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Aug 24 02:12:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 24 02:11:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	124460	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	128934	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	56633	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35547	4.013	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	80.200%	
7) Chloroethane-d5	1.564	69	39921	6.158	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	123.200%	
11) 1,1-Dichloroethene-d2	2.105	63	71561	3.465	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.200%	
20) 2-Butanone-d5	3.895	46	37861	34.346	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	68.700%	
24) Chloroform-d	4.346	84	79891	4.511	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
26) 1,2-Dichloroethane-d4	5.027	65	36435	4.755	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.200%	
32) Benzene-d6	5.047	84	150139	4.204	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.000%	
36) 1,2-Dichloropropane-d6	6.066	67	44704	4.306	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.200%	
41) Toluene-d8	7.313	98	118006	3.660	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	73.200%	
43) trans-1,3-Dichloroprop...	7.625	79	14404	4.052	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.000%	
46) 2-Hexanone-d5	8.091	63	44626	38.134	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	76.260%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30865	4.668	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	39822	4.743	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	3587	0.253	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
Data File : VV027482.D
Acq On : 23 Aug 2022 12:26
Operator : SY/MD
Sample : N4253-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Aug 24 02:12:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 24 02:11:24 2022
Response via : Initial Calibration

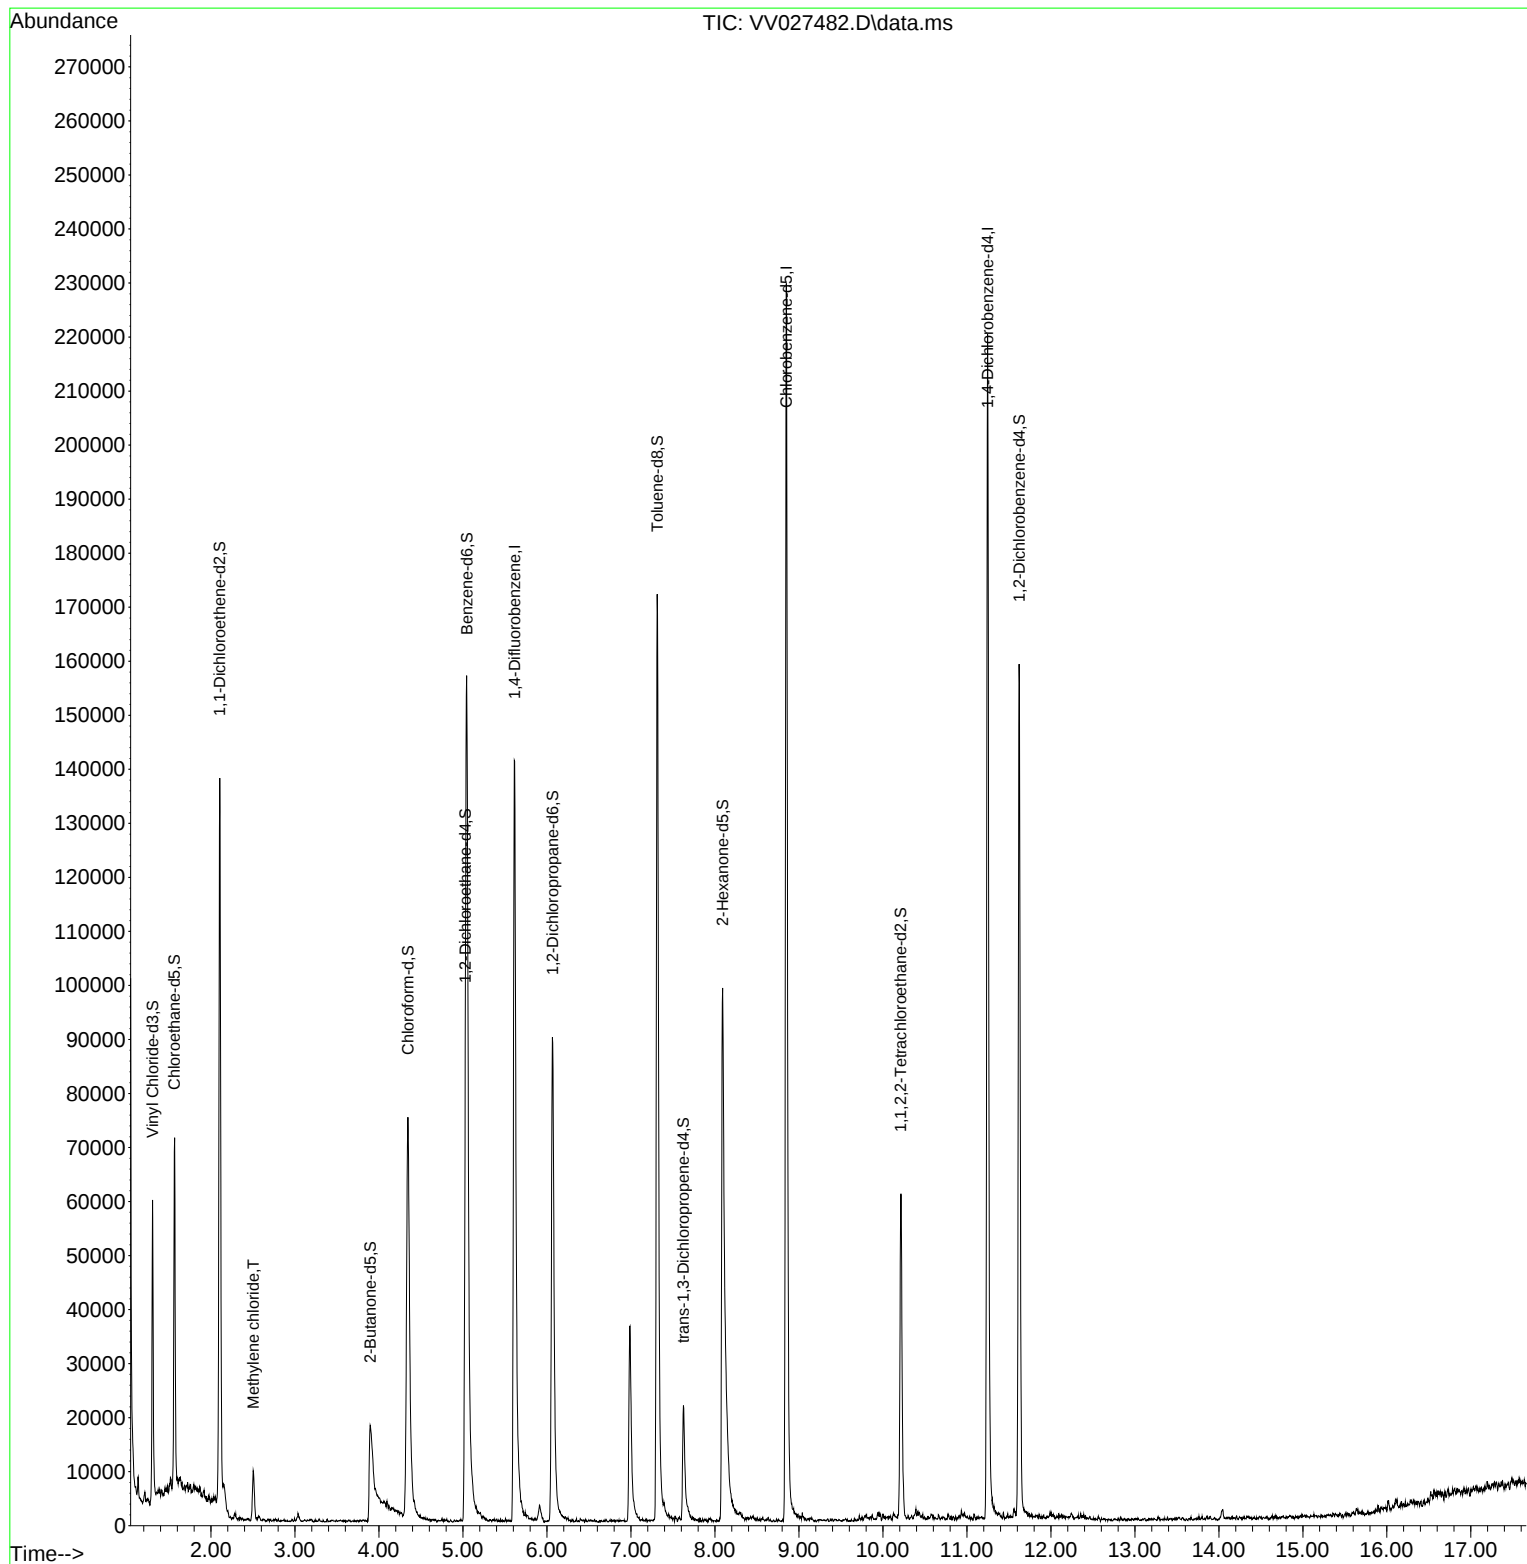

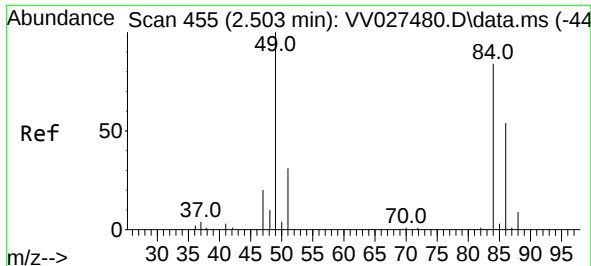

#16
Methylene chloride
Concen: 0.253 ug/L
RT: 2.503 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV027482.D
Acq: 23 Aug 2022 12:26

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

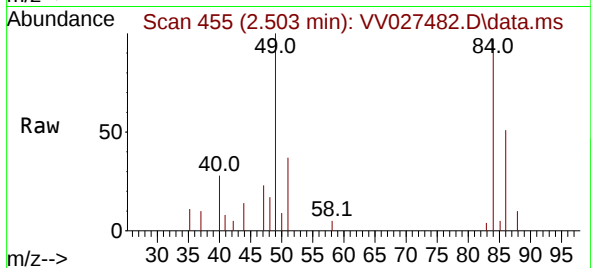

Tgt Ion: 84 Resp: 3587

Ion	Ratio	Lower	Upper
84	100		
86	52.7	44.0	81.6
49	102.9	89.4	166.0

