

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
 Data File : VV027483.D
 Acq On : 23 Aug 2022 12:53
 Operator : SY/MD
 Sample : N4252-05DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9C6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	48	54	61	rBV2	6593	6927	1.51%	0.186%
2	1.307	72	83	97	rBV2	98483	118996	25.87%	3.194%
3	1.565	156	163	172	rVB	59337	67556	14.69%	1.813%
4	2.105	321	331	341	rBV	135100	193230	42.02%	5.187%
5	2.503	446	455	468	rBV2	15911	27213	5.92%	0.730%
6	2.761	522	535	548	rBV2	10264	18574	4.04%	0.499%
7	3.905	875	891	930	rBV2	158562	459888	100.00%	12.345%
8	4.346	1011	1028	1061	rBV	72234	193648	42.11%	5.198%
9	5.044	1231	1245	1281	rBV4	154223	409884	89.13%	11.003%
10	5.616	1411	1423	1457	rBV	133884	297279	64.64%	7.980%
11	5.915	1506	1516	1529	rBV7	9823	22398	4.87%	0.601%
12	6.066	1551	1563	1593	rBV	90952	201375	43.79%	5.406%
13	6.986	1840	1849	1869	rBV2	36983	73777	16.04%	1.980%
14	7.314	1941	1951	1973	rBV	168074	314155	68.31%	8.433%
15	7.625	2039	2048	2064	rBV2	21999	40924	8.90%	1.099%
16	8.092	2184	2193	2225	rBV2	101672	255561	55.57%	6.860%
17	8.850	2417	2429	2446	rBV	217770	363513	79.04%	9.758%
18	10.214	2842	2853	2870	rBV	56730	92361	20.08%	2.479%
19	11.246	3163	3174	3188	rBV	206605	327605	71.24%	8.794%
20	11.622	3280	3291	3309	rBV	147255	240492	52.29%	6.456%




Sum of corrected areas: 3725356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
Data File : VV027483.D
Acq On : 23 Aug 2022 12:53
Operator : SY/MD
Sample : N4252-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

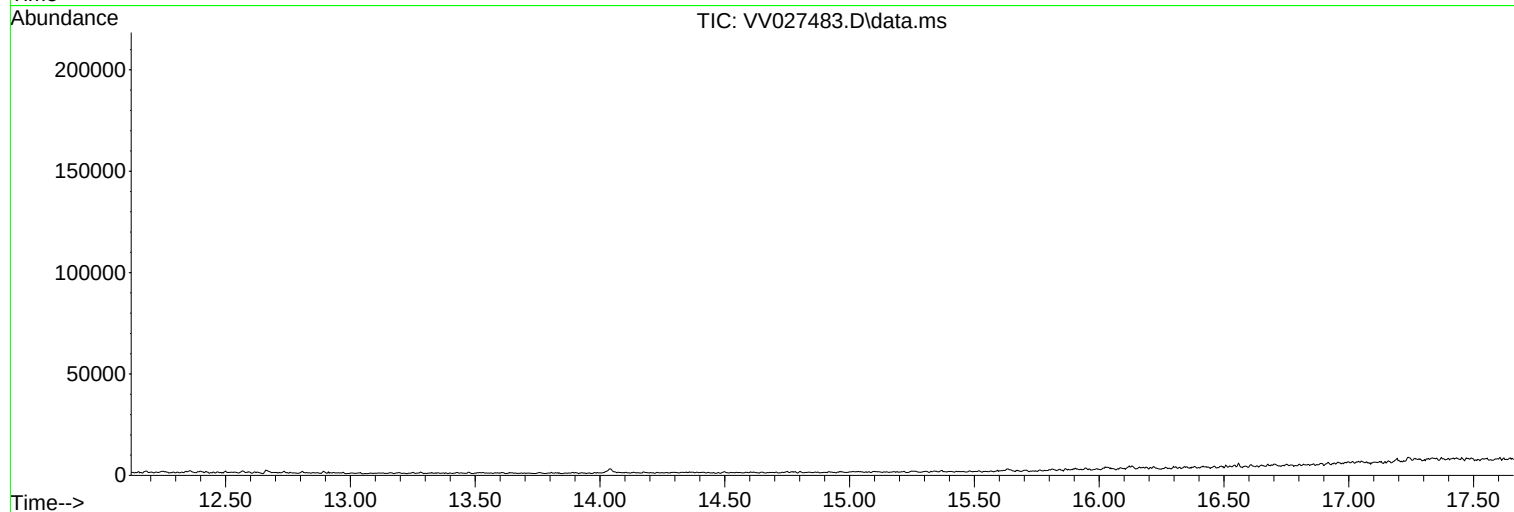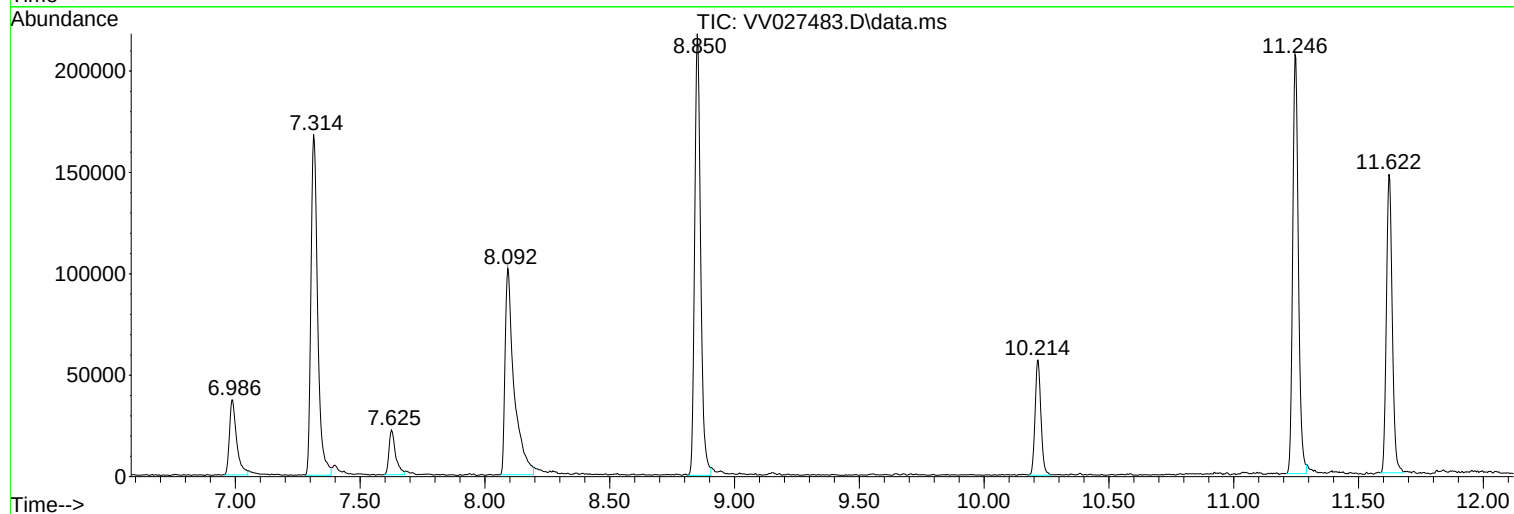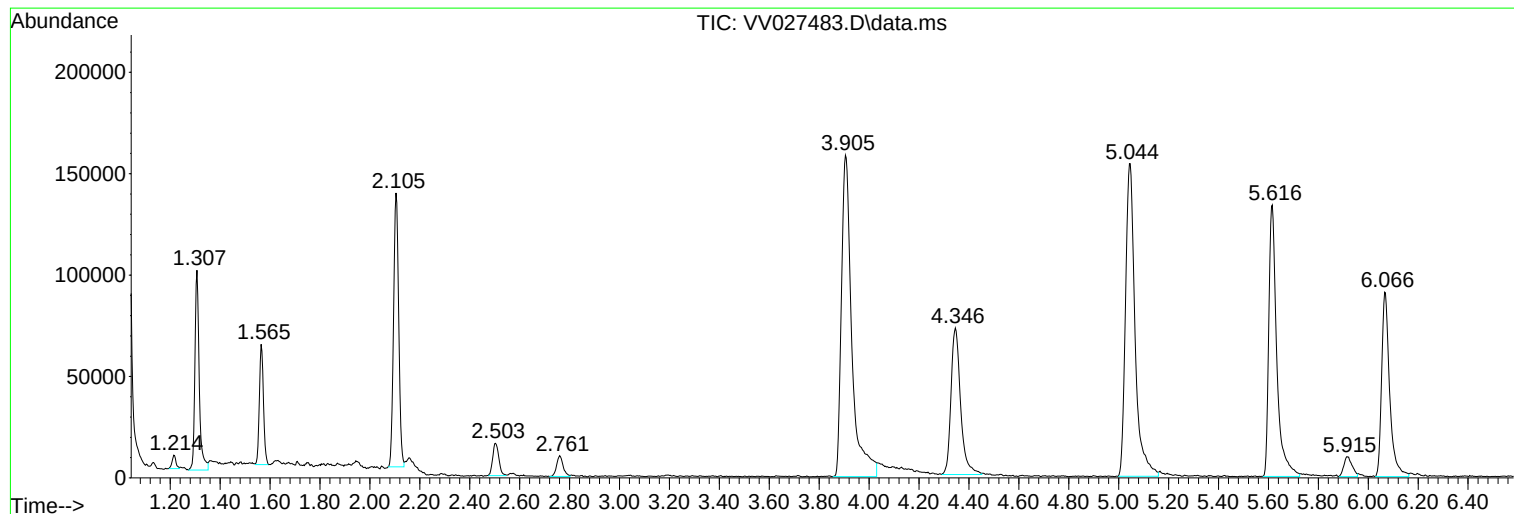

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
Data File : VV027483.D
Acq On : 23 Aug 2022 12:53
Operator : SY/MD
Sample : N4252-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
Data File : VV027483.D
Acq On : 23 Aug 2022 12:53
Operator : SY/MD
Sample : N4252-05DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------