


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082322\
Data File : VV027479.D
Acq On : 23 Aug 2022 09:22
Operator : SY/MD
Sample : BFB358
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB358

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Aug 25 06:25:30 2022

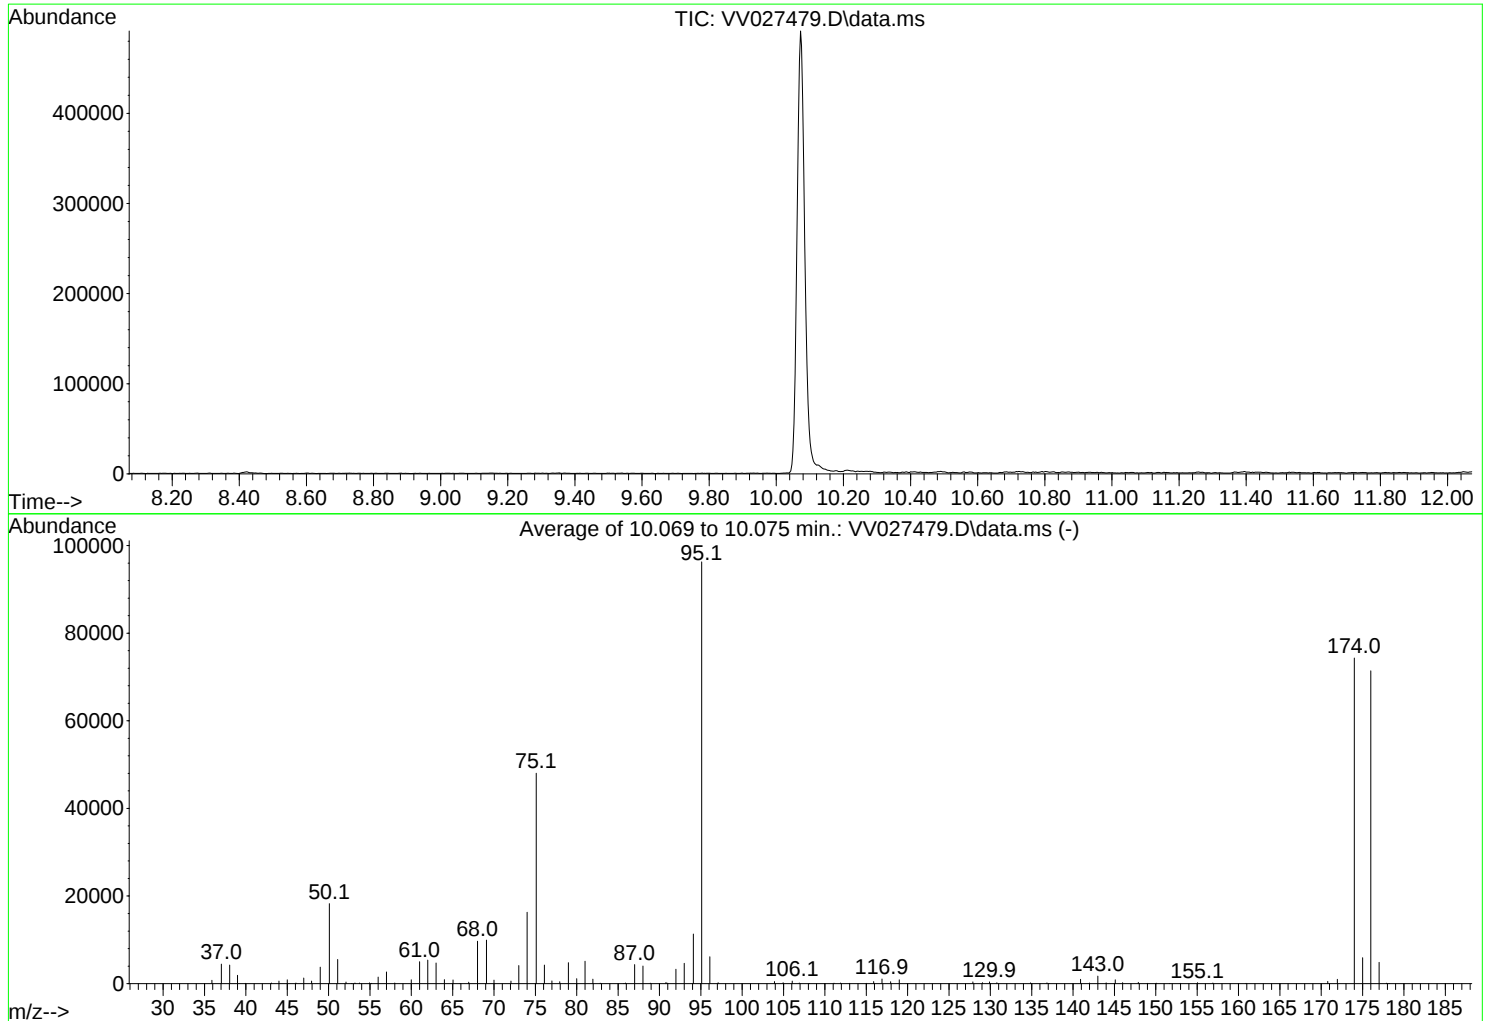

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	18261	PASS
75	95	30	80	49.9	48045	PASS
95	95	100	100	100.0	96293	PASS
96	95	5	9	6.4	6134	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.2	74323	PASS
175	174	5	9	8.0	5909	PASS
176	174	95	105	96.1	71405	PASS
177	176	5	10	6.8	4874	PASS

Scan 2796 (10.030 min): VV027479.D\data.ms
BFB358

m/z	Abundance
35.80	113.0
40.00	408.0
44.00	453.0
79.20	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	865.0
37.10	4451.0
38.00	4282.0
39.00	1918.0
39.90	434.0
43.20	158.0
44.00	1035.0
45.00	897.0
46.10	251.0
47.00	1240.0
47.90	545.0
49.00	3870.0
50.10	18320.0
51.10	5536.0
52.10	389.0
53.20	204.0
53.80	142.0
55.20	244.0
56.00	1401.0
57.00	2461.0
57.90	164.0
60.00	935.0
61.00	5169.0
62.00	5335.0
63.00	4542.0
64.00	896.0
65.00	808.0
66.90	300.0
68.00	9371.0
69.10	9734.0
70.00	761.0
72.10	603.0
73.00	4095.0
74.00	16118.0
75.10	47112.0
76.10	4167.0
77.00	561.0
77.90	419.0
79.00	4722.0
80.00	1061.0
81.00	5112.0
82.00	920.0
82.80	104.0
85.70	123.0
87.00	4210.0
88.00	3811.0
90.80	472.0
92.00	3138.0
93.00	4673.0
94.10	10730.0
95.10	93480.0
96.10	6029.0
97.10	179.0
103.90	450.0
104.90	190.0
106.00	444.0
106.90	178.0
110.00	111.0
111.20	103.0
111.80	132.0
115.90	449.0
116.90	906.0
117.90	398.0
119.00	851.0
127.90	382.0
129.10	200.0
129.90	392.0
130.80	236.0
134.90	192.0
136.90	198.0
140.90	865.0
142.00	129.0
143.00	1663.0
144.00	207.0
145.10	789.0
146.00	201.0
147.90	273.0
150.10	103.0
151.70	103.0
153.00	153.0
155.00	251.0
156.90	126.0
170.80	473.0
171.90	890.0
174.00	69696.0
175.00	5689.0
176.00	66912.0
177.00	4613.0
177.90	206.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	926.0
37.00	4585.0
38.00	4380.0
39.00	1896.0
40.00	480.0
43.10	141.0
44.10	1057.0
45.00	880.0
47.00	1323.0
48.00	615.0
49.00	3933.0
50.10	18968.0
51.10	5702.0
52.10	395.0
53.20	195.0
53.70	155.0
54.90	269.0
56.00	1526.0
57.00	2746.0
58.00	146.0
60.00	864.0
61.00	5110.0
62.00	5585.0
63.00	4853.0
64.00	933.0
65.10	825.0
67.00	332.0
68.00	10100.0
69.10	10333.0
70.00	849.0
72.10	630.0
73.00	4276.0
74.00	16984.0
75.10	49728.0
76.10	4379.0
77.00	650.0
77.90	477.0
79.00	5109.0
80.00	1171.0
81.00	5250.0
81.90	1057.0
82.90	107.0
85.90	199.0
87.00	4580.0
88.00	4167.0
88.90	172.0
90.80	417.0
92.00	3438.0
93.00	4782.0
94.10	11828.0
95.10	99576.0
96.10	6367.0
97.10	226.0
103.90	500.0
105.00	221.0
106.10	468.0
106.90	174.0
111.10	132.0
111.90	134.0
113.00	112.0
115.00	105.0
115.90	470.0
116.90	1112.0
118.00	440.0
119.00	899.0
127.90	421.0
129.10	224.0
129.90	418.0
130.80	225.0
134.90	169.0
136.90	196.0
140.90	1029.0
142.00	174.0
143.00	1741.0
144.00	176.0
145.10	928.0
146.00	216.0
147.90	300.0
149.00	136.0
150.10	137.0
152.90	114.0
155.10	224.0
156.90	153.0
161.00	101.0
170.80	521.0
171.90	1021.0
174.00	76904.0
175.00	6131.0
176.00	74048.0
177.00	5027.0
177.90	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
36.00	833.0
37.00	4295.0
38.10	4082.0
39.00	1855.0
40.00	517.0
43.00	119.0
44.00	980.0
45.00	829.0
46.00	196.0
47.00	1317.0
48.00	630.0
49.00	3499.0
50.10	17496.0
51.10	5324.0
52.10	356.0
52.80	166.0
53.70	158.0
55.00	265.0
56.00	1625.0
57.00	2767.0
58.10	124.0
60.00	833.0
61.00	4690.0
62.00	5171.0
63.00	4729.0
64.00	968.0
65.10	860.0
65.90	132.0
67.00	325.0
68.00	9537.0
69.10	9731.0
70.00	810.0
72.00	540.0
73.00	4015.0
74.00	15824.0
75.10	47296.0
76.10	4142.0
77.00	621.0
78.00	440.0
79.00	4854.0
80.00	1158.0
81.00	4989.0
81.90	1078.0
82.90	130.0
85.90	235.0
87.00	4252.0
88.00	4048.0
88.90	157.0
91.00	355.0
92.00	3273.0
93.00	4498.0
94.10	11435.0
95.10	95824.0
96.10	6005.0
97.10	229.0
103.90	461.0
105.00	210.0
105.90	413.0
106.10	418.0
106.90	142.0
108.10	118.0
111.00	129.0
112.00	130.0
112.90	158.0
115.00	134.0
115.90	461.0
116.90	1171.0
117.90	439.0
119.00	833.0
127.90	381.0
129.00	206.0
129.90	379.0
130.80	165.0
134.80	159.0
136.70	169.0
137.10	139.0
140.90	1024.0
142.00	175.0
143.00	1769.0
144.00	141.0
145.10	948.0
146.00	215.0
147.90	271.0
149.00	124.0
150.00	136.0
155.00	195.0
156.90	168.0
160.80	110.0
170.80	510.0
172.00	1045.0
174.00	76368.0
175.00	5907.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

176.00	73256.0
177.00	4983.0
178.20	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358