




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031867.D
 Acq On : 23 Aug 2023 14:03
 Operator : SY/MD
 Sample : 04034-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN6

Manual IntegrationsAPPROVED

Quant Time: Aug 24 01:57:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/24/2023
 Supervised By :Mahesh Dadoda 08/24/2023

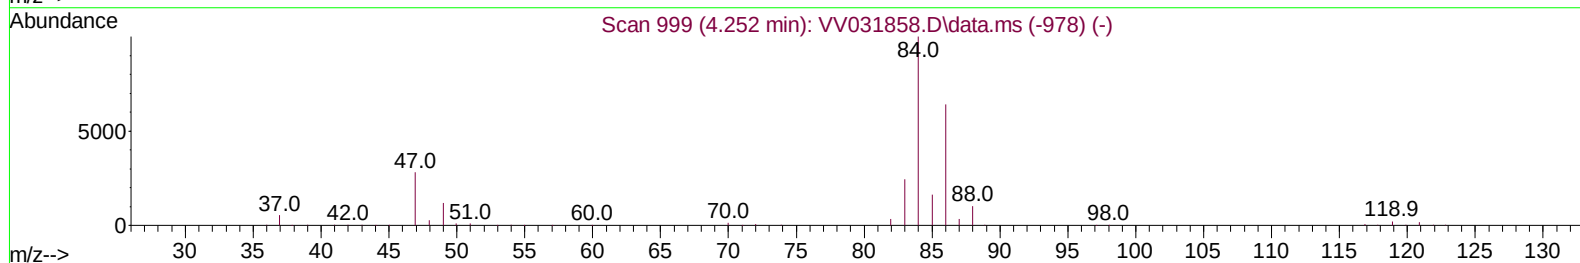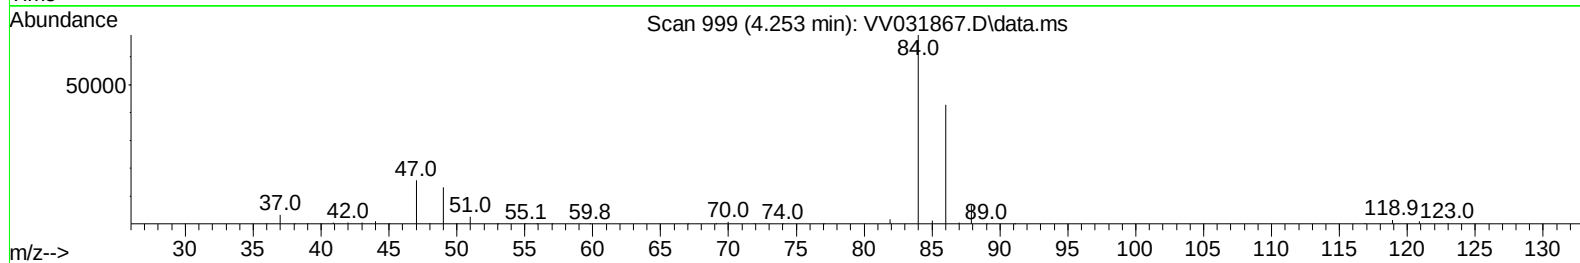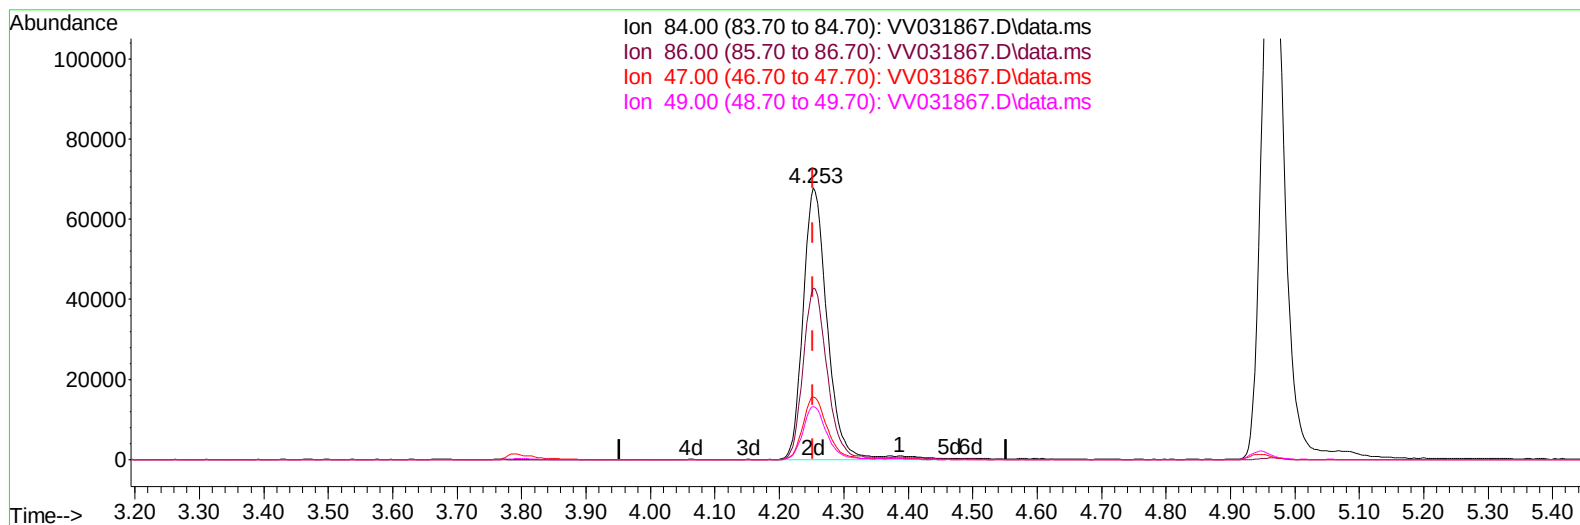

TIC: VV031867.D\data.ms

(24) Chloroform-d (S)

4.253min (+ 0.001) 47.52 ug/L m

response 177224

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	0.03#
47.00	45.70	0.03#
49.00	27.00	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031867.D
 Acq On : 23 Aug 2023 14:03
 Operator : SY/MD
 Sample : 04034-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN6

Manual IntegrationsAPPROVED

Quant Time: Aug 24 01:57:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/24/2023
 Supervised By :Mahesh Dadoda 08/24/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.539	114		272630	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117		268081	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		142252	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		77203	45.248	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	90.500%	
7) Chloroethane-d5	1.532	69		71222	47.618	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	95.240%	
11) 1,1-Dichloroethene-d2	2.060	65		36413	45.577	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	91.160%	
21) 2-Butanone-d5	3.790	46		127852	95.274	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	95.270%	
24) Chloroform-d	4.253	84		177224m	47.522	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	95.040%	
26) 1,2-Dichloroethane-d4	4.947	65		118592	47.918	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	95.840%	
32) Benzene-d6	4.963	84		357266	48.839	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	97.680%	
36) 1,2-Dichloropropane-d6	5.992	67		115152	48.907	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	97.820%	
41) Toluene-d8	7.246	98		325040	48.224	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	96.440%	
43) trans-1,3-Dichloroprop...	7.558	79		58880	48.248	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	96.500%	
47) 2-Hexanone-d5	8.031	63		64684	89.634	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	89.630%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		137015	45.033	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	90.060%	
66) 1,2-Dichlorobenzene-d4	11.564	152		128098	49.398	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	98.800%	
Target Compounds							
13) Acetone	2.118	43		9969	8.346	ug/L	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031867.D
Acq On : 23 Aug 2023 14:03
Operator : SY/MD
Sample : 04034-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYIN6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/24/2023
Supervised By :Mahesh Dadoda 08/24/2023

Quant Time: Aug 24 01:57:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 24 01:40:47 2023
Response via : Initial Calibration

