




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031873.D
 Acq On : 23 Aug 2023 16:22
 Operator : SY/MD
 Sample : 04037-09ME
 Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYJ3ME

Manual IntegrationsAPPROVED

Quant Time: Aug 24 01:58:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/24/2023
 Supervised By :Mahesh Dadoda 08/24/2023

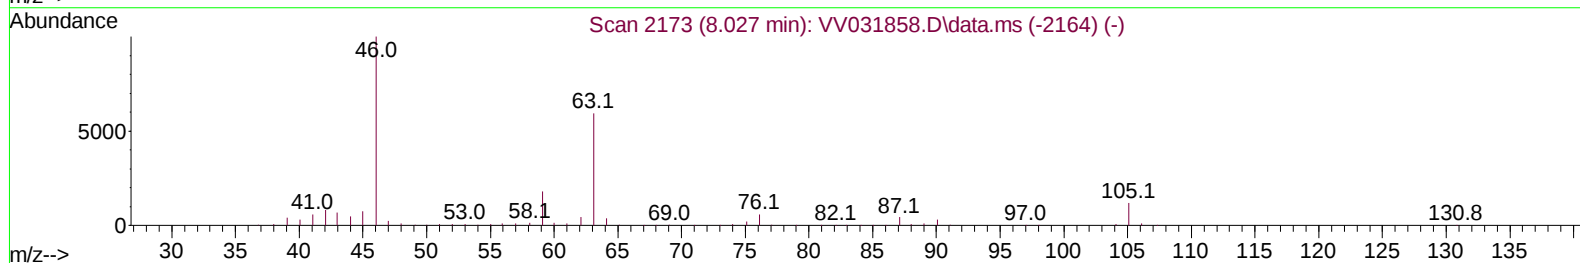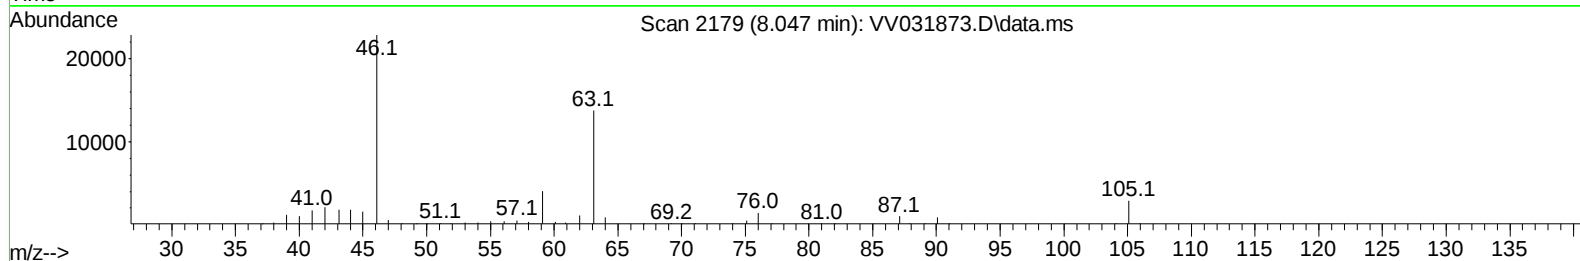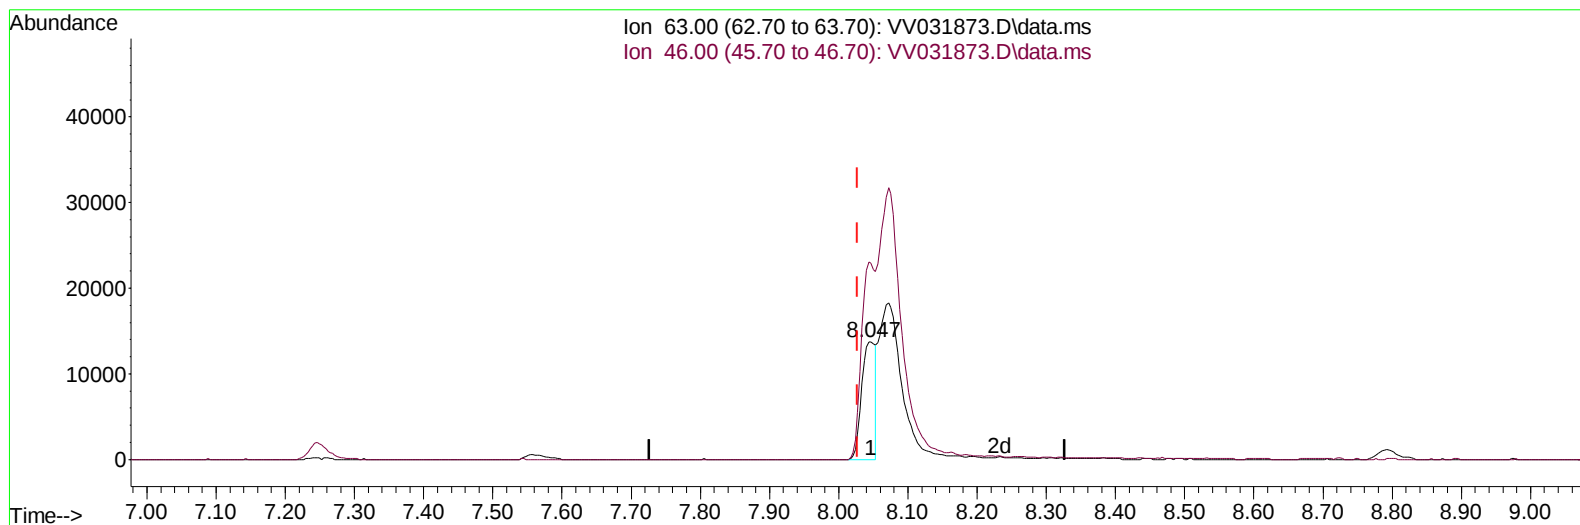

TIC: VV031873.D\data.ms

(47) 2-Hexanone-d5 (S)

8.047min (+ 0.020) 24.53 ug/L

response 18970

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	169.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031873.D
Acq On : 23 Aug 2023 16:22
Operator : SY/MD
Sample : 04037-09ME
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYJ3ME

Manual IntegrationsAPPROVED

Quant Time: Aug 24 01:58:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 24 01:40:47 2023
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/24/2023
Supervised By :Mahesh Dadoda 08/24/2023

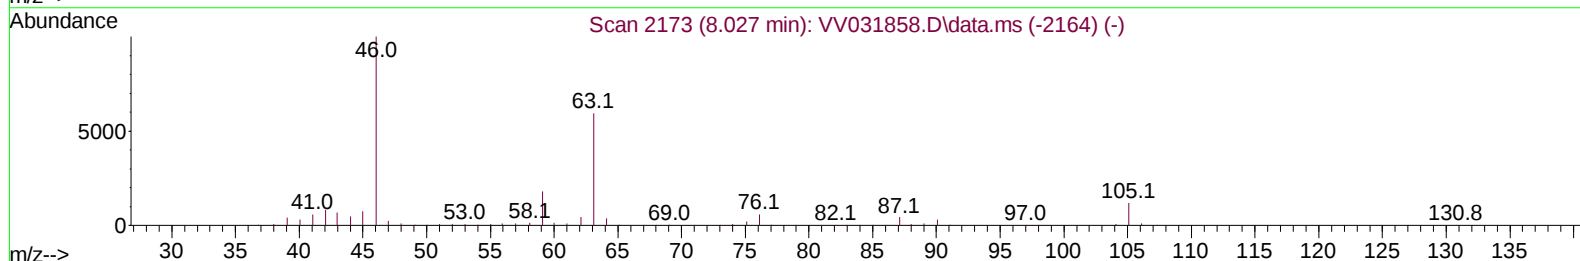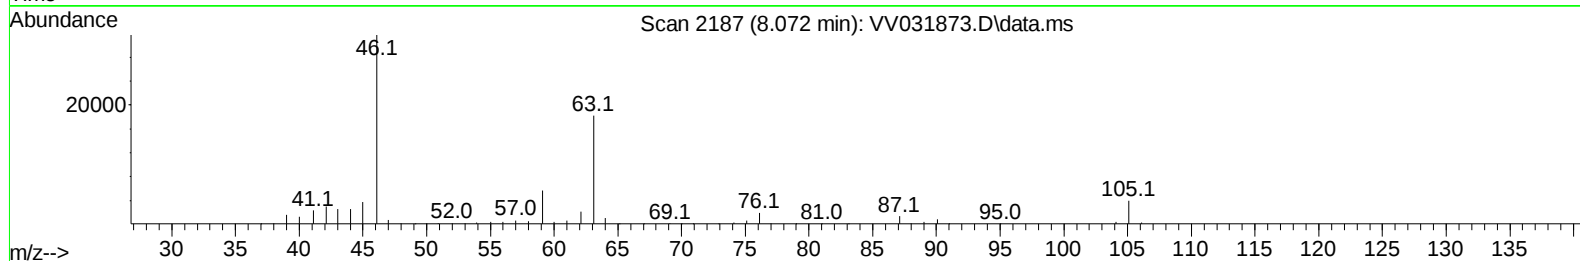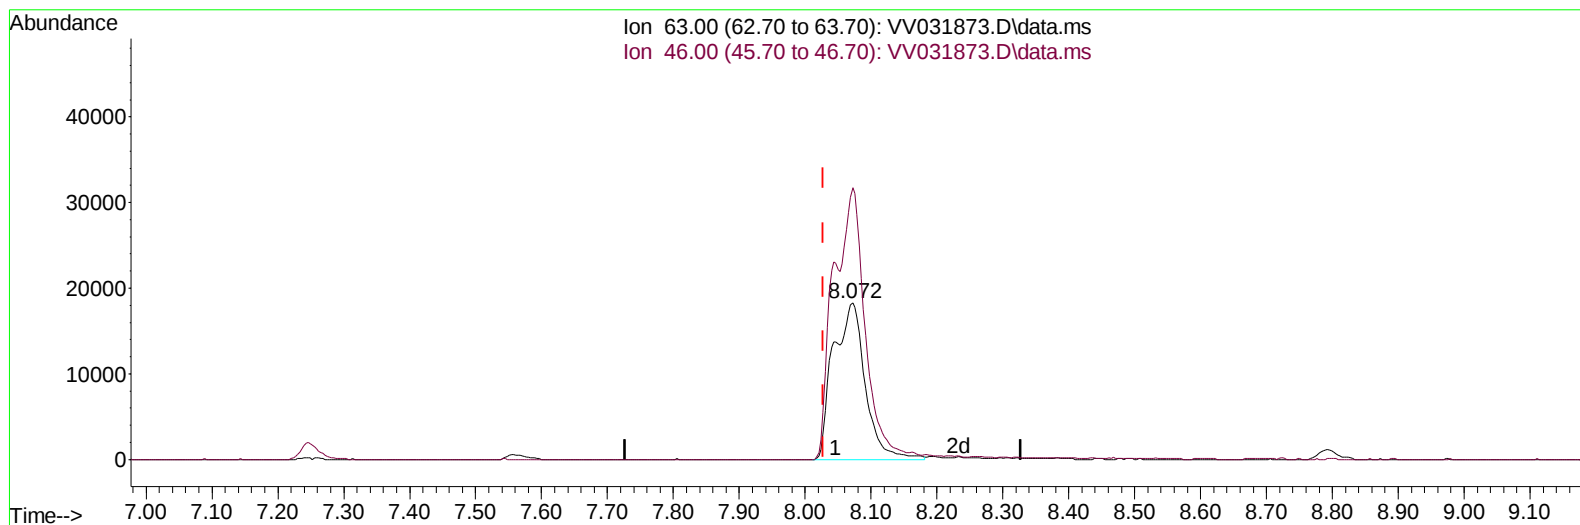

TIC: VV031873.D\data.ms

(47) 2-Hexanone-d5 (S)

8.072min (+ 0.045) 79.34 ug/L m

response 61371

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	52.29#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031873.D
 Acq On : 23 Aug 2023 16:22
 Operator : SY/MD
 Sample : 04037-09ME
 Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYJ3ME

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/24/2023
 Supervised By :Mahesh Dadoda 08/24/2023

Quant Time: Aug 24 01:58:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	295826	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	287336	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	148202	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	69353	37.460	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	74.920%	
7) Chloroethane-d5	1.529	69	45121	27.802	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	55.600%#	
11) 1,1-Dichloroethene-d2	2.040	65	32478	37.464	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	74.920%	
21) 2-Butanone-d5	3.818	46	110338	75.776	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	75.780%	
24) Chloroform-d	4.252	84	161666	39.951	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.900%	
26) 1,2-Dichloroethane-d4	4.944	65	111967	41.693	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.380%	
32) Benzene-d6	4.960	84	337726	43.074	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.140%	
36) 1,2-Dichloropropane-d6	5.992	67	111354	44.125	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	88.240%	
41) Toluene-d8	7.246	98	306472	42.422	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.840%	
43) trans-1,3-Dichloroprop...	7.558	79	59184	45.247	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	90.500%	
47) 2-Hexanone-d5	8.072	63	61371m	79.344	ug/L	0.05
Spiked Amount 100.000	Range 45	- 130	Recovery	=	79.340%	
56) 1,1,2,2-Tetrachloroeth...	10.165	84	138759	42.550	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.100%	
66) 1,2-Dichlorobenzene-d4	11.570	152	119254	44.141	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	88.280%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031873.D
Acq On : 23 Aug 2023 16:22
Operator : SY/MD
Sample : 04037-09ME
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYJ3ME

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/24/2023
Supervised By :Mahesh Dadoda 08/24/2023

Quant Time: Aug 24 01:58:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 24 01:40:47 2023
Response via : Initial Calibration

