

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW082323\
 Data File : VW031864.D
 Acq On : 23 Aug 2023 12:56
 Operator : SY/MD
 Sample : 04034-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN5

Quant Time: Aug 24 01:56:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	278819	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	276839	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	144278	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	78532	45.005	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.020%
7) Chloroethane-d5	1.532	69	70068	45.806	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.620%
11) 1,1-Dichloroethene-d2	2.060	65	37253	45.593	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.180%
21) 2-Butanone-d5	3.786	46	126988	92.530	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.530%
24) Chloroform-d	4.252	84	173571	45.509	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.020%
26) 1,2-Dichloroethane-d4	4.947	65	117533	46.436	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.880%
32) Benzene-d6	4.963	84	356913	47.247	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.500%
36) 1,2-Dichloropropane-d6	5.992	67	115546	47.522	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.040%
41) Toluene-d8	7.246	98	327087	46.993	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.980%
43) trans-1,3-Dichloroprop...	7.558	79	58860	46.706	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.420%
47) 2-Hexanone-d5	8.030	63	63522	85.239	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.240%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	139391	44.364	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.720%
66) 1,2-Dichlorobenzene-d4	11.564	152	127024	48.296	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.600%
Target Compounds						
13) Acetone	2.114	43	10127	8.291	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031864.D
Acq On : 23 Aug 2023 12:56
Operator : SY/MD
Sample : 04034-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN5

Quant Time: Aug 24 01:56:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 24 01:40:47 2023
Response via : Initial Calibration

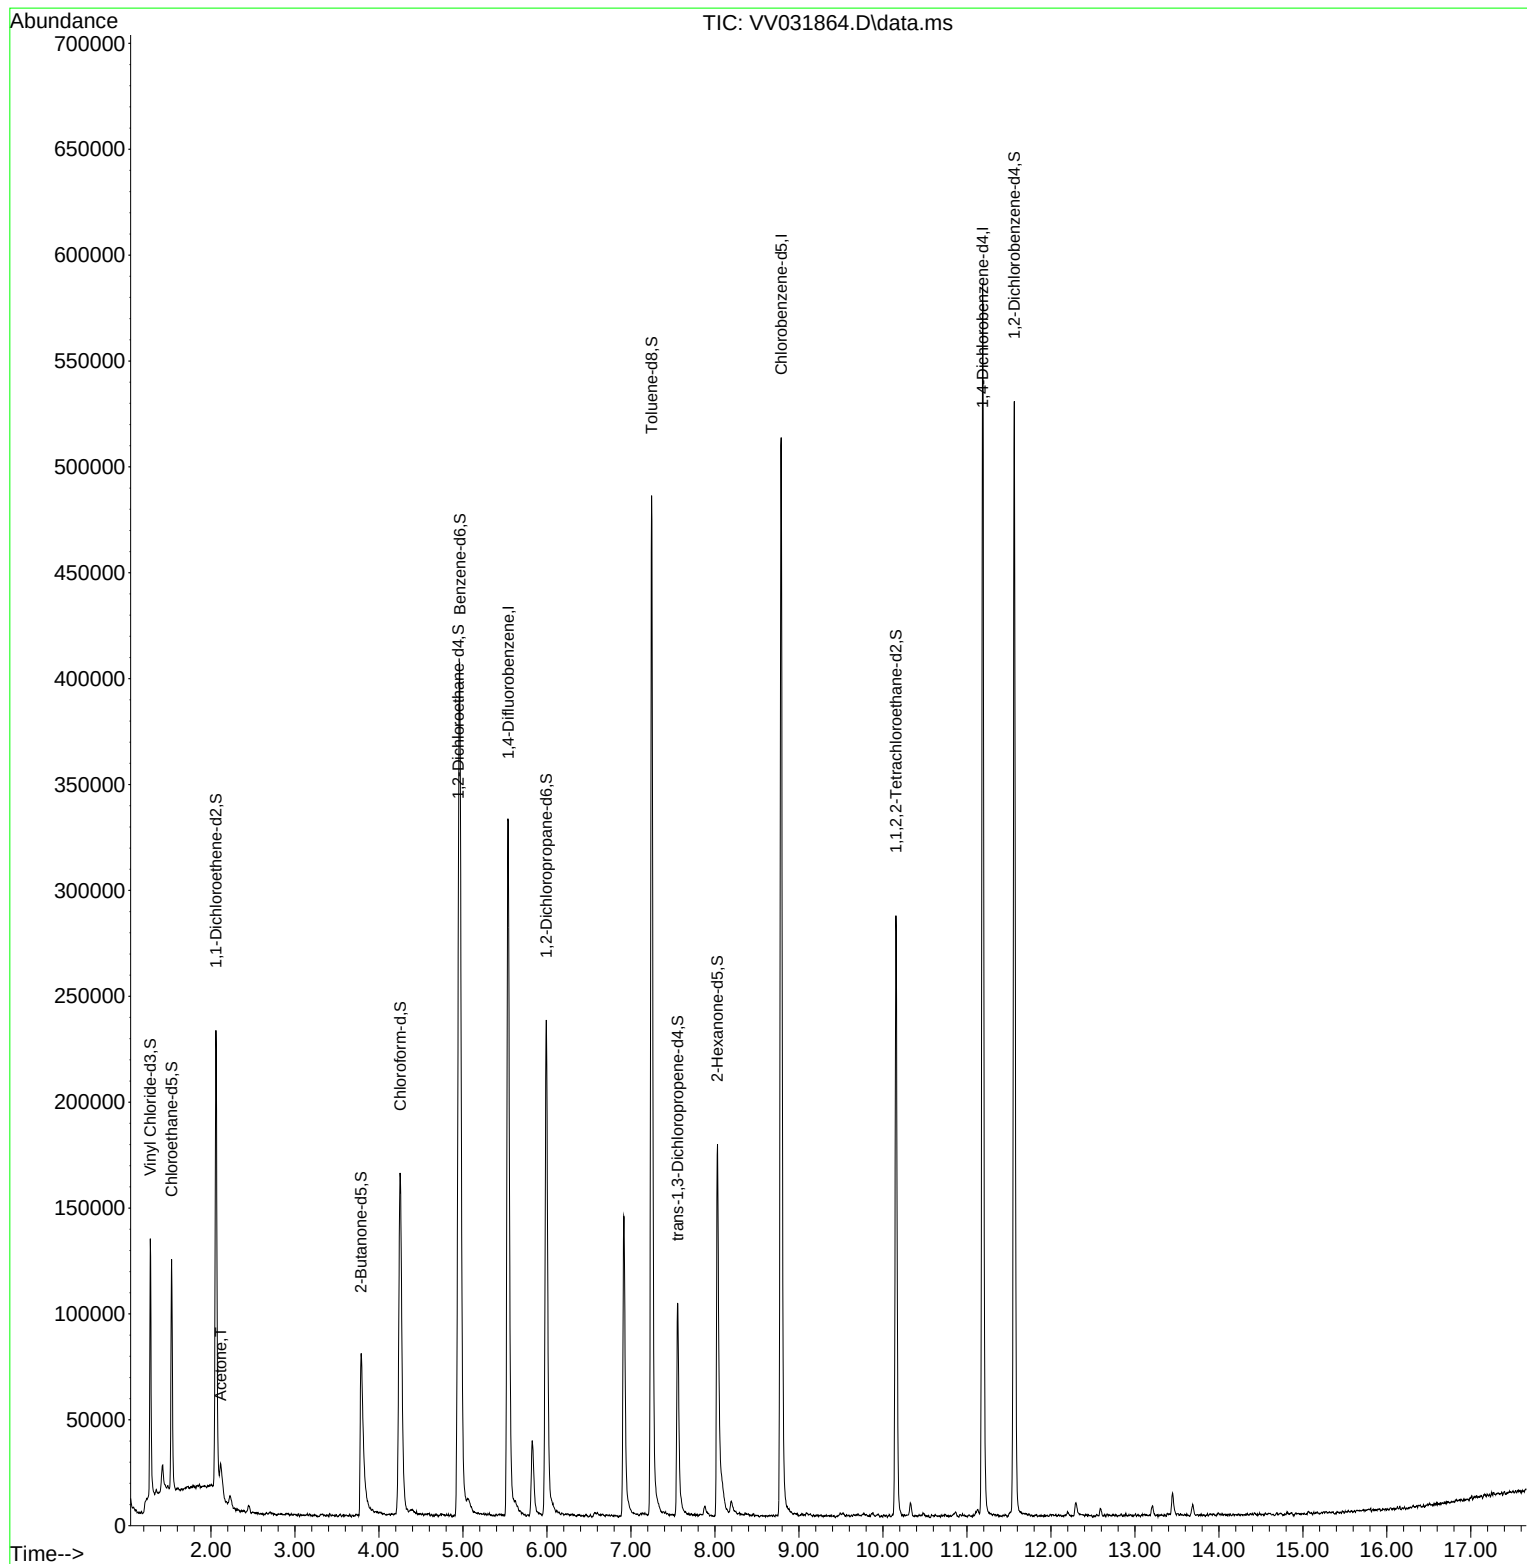

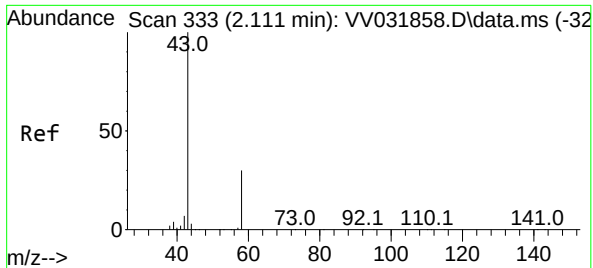

#13
 Acetone
 Concen: 8.291 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV031864.D
 Acq: 23 Aug 2023 12:56

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN5

Tgt Ion: 43 Resp: 10127
 Ion Ratio Lower Upper
 43 100
 58 22.9 0.0 61.0

