

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW082323\
 Data File : VW031865.D
 Acq On : 23 Aug 2023 13:19
 Operator : SY/MD
 Sample : 04034-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR0

Quant Time: Aug 24 01:56:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	270756	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	265523	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	140131	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	77567	45.776	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.560%
7) Chloroethane-d5	1.532	69	71462	48.109	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.220%
11) 1,1-Dichloroethene-d2	2.059	65	36631	46.167	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.340%
21) 2-Butanone-d5	3.786	46	133556	100.214	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.210%
24) Chloroform-d	4.252	84	171171	46.216	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.440%
26) 1,2-Dichloroethane-d4	4.944	65	117597	47.845	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.680%
32) Benzene-d6	4.963	84	353363	48.771	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.540%
36) 1,2-Dichloropropane-d6	5.992	67	114940	49.287	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.580%
41) Toluene-d8	7.246	98	325579	48.769	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.540%
43) trans-1,3-Dichloroprop...	7.558	79	59196	48.974	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.940%
47) 2-Hexanone-d5	8.030	63	66711	93.333	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.330%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	138465	45.948	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.900%
66) 1,2-Dichlorobenzene-d4	11.564	152	127037	49.730	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.460%
Target Compounds						
13) Acetone	2.114	43	9941	8.381	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031865.D
Acq On : 23 Aug 2023 13:19
Operator : SY/MD
Sample : 04034-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR0

Quant Time: Aug 24 01:56:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 24 01:40:47 2023
Response via : Initial Calibration

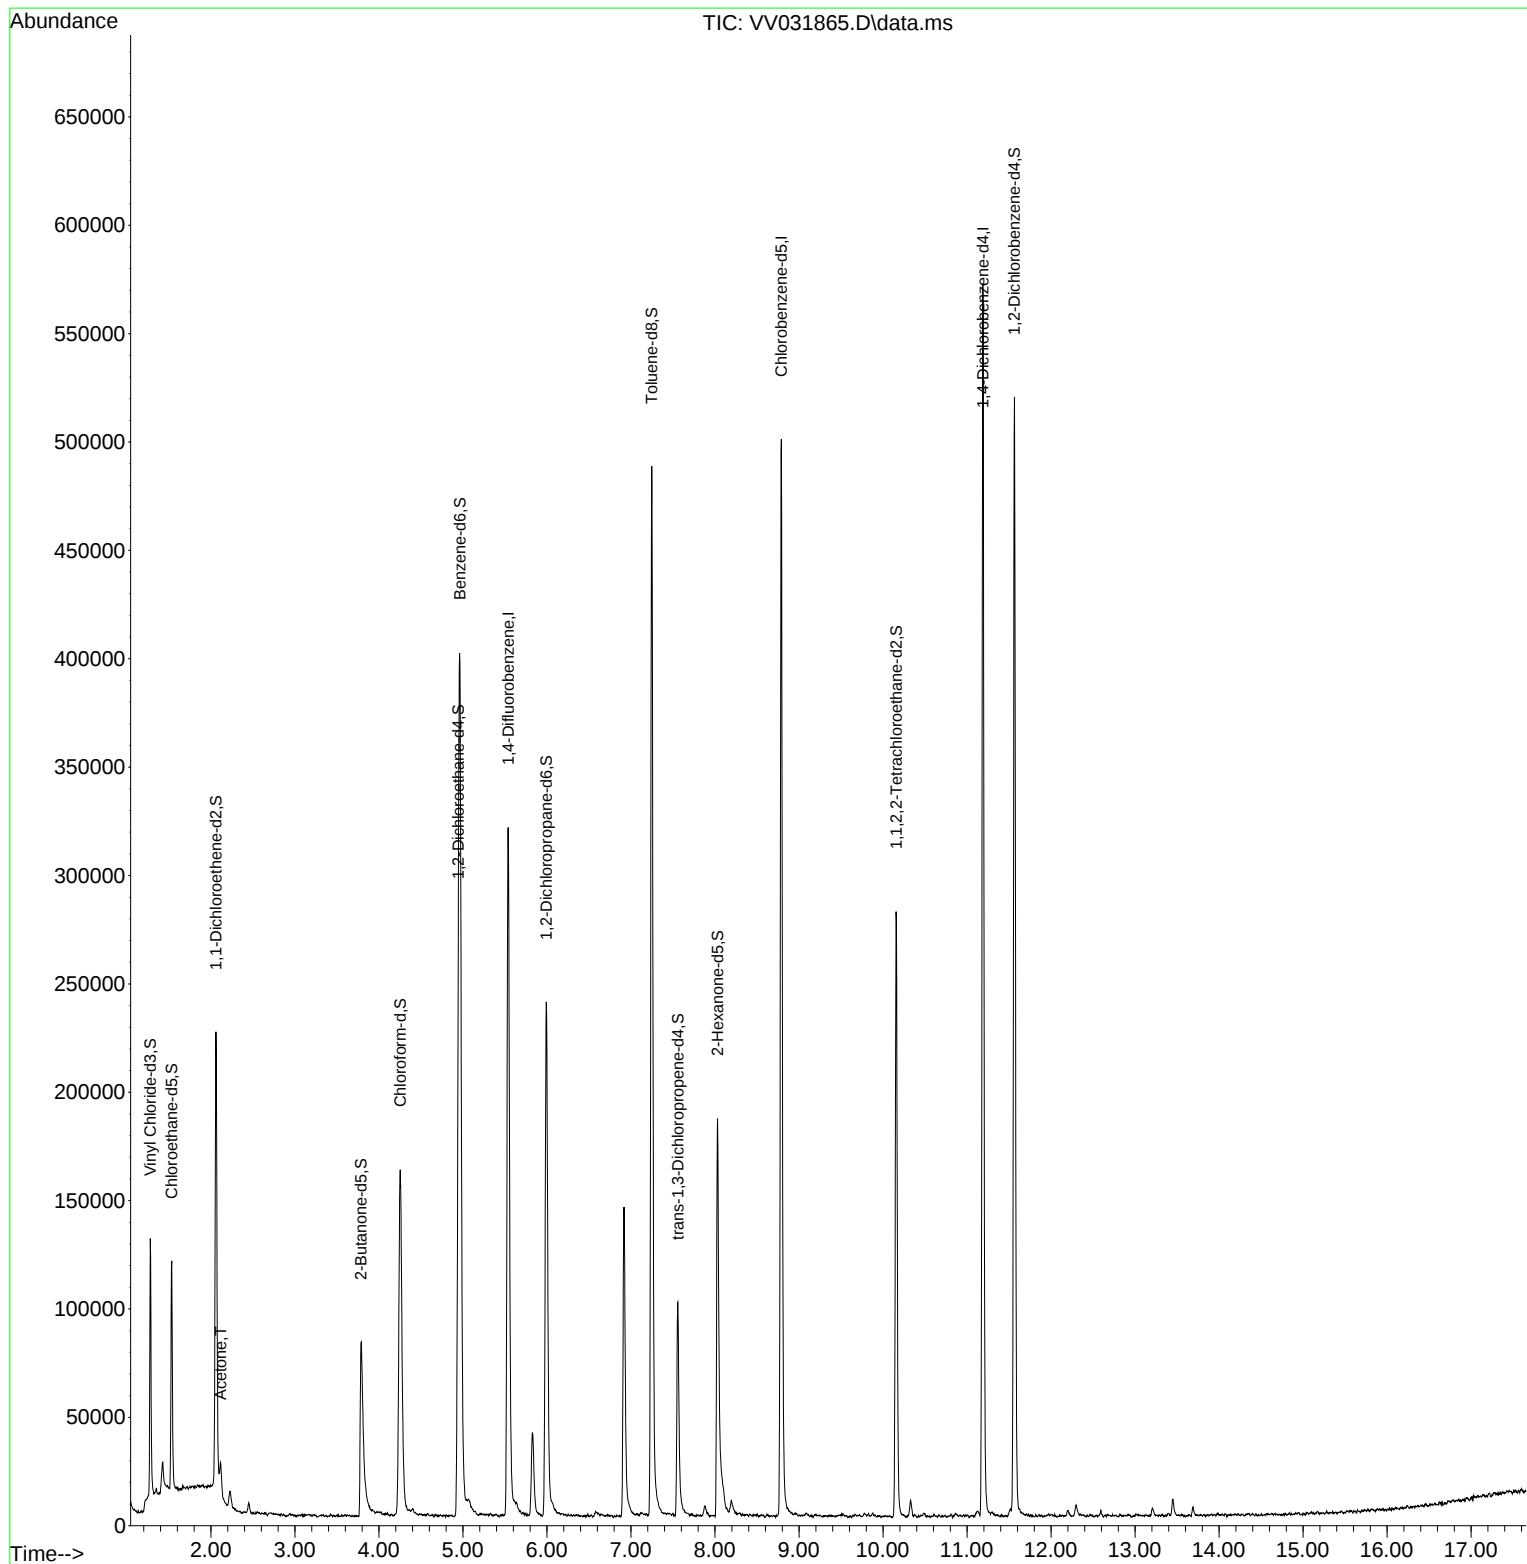

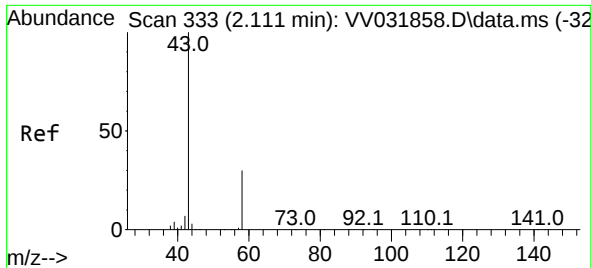

#13
 Acetone
 Concen: 8.381 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV031865.D
 Acq: 23 Aug 2023 13:19

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR0

Tgt Ion: 43 Resp: 9941
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 61.0

