

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW082323\
 Data File : VW031871.D
 Acq On : 23 Aug 2023 15:35
 Operator : SY/MD
 Sample : 04037-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN7

Quant Time: Aug 24 01:58:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 24 01:40:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	266693	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	256859	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	137265	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	72895	43.674	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.340%
7) Chloroethane-d5	1.532	69	66304	45.317	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.640%
11) 1,1-Dichloroethene-d2	2.063	65	35637	45.598	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.200%
21) 2-Butanone-d5	3.796	46	128118	97.598	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.600%
24) Chloroform-d	4.256	84	167553	45.929	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.860%
26) 1,2-Dichloroethane-d4	4.947	65	112321	46.394	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.780%
32) Benzene-d6	4.966	84	344755	49.188	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.380%
36) 1,2-Dichloropropane-d6	5.992	67	113270	50.210	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.420%
41) Toluene-d8	7.246	98	310508	48.081	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.160%
43) trans-1,3-Dichloroprop...	7.558	79	55998	47.891	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.780%
47) 2-Hexanone-d5	8.031	63	62741	90.740	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.740%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	130421	44.738	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.480%
66) 1,2-Dichlorobenzene-d4	11.564	152	125389	50.110	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.220%
Target Compounds						
13) Acetone	2.124	43	7728	6.614	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031871.D
Acq On : 23 Aug 2023 15:35
Operator : SY/MD
Sample : 04037-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY7

Quant Time: Aug 24 01:58:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 24 01:40:47 2023
Response via : Initial Calibration

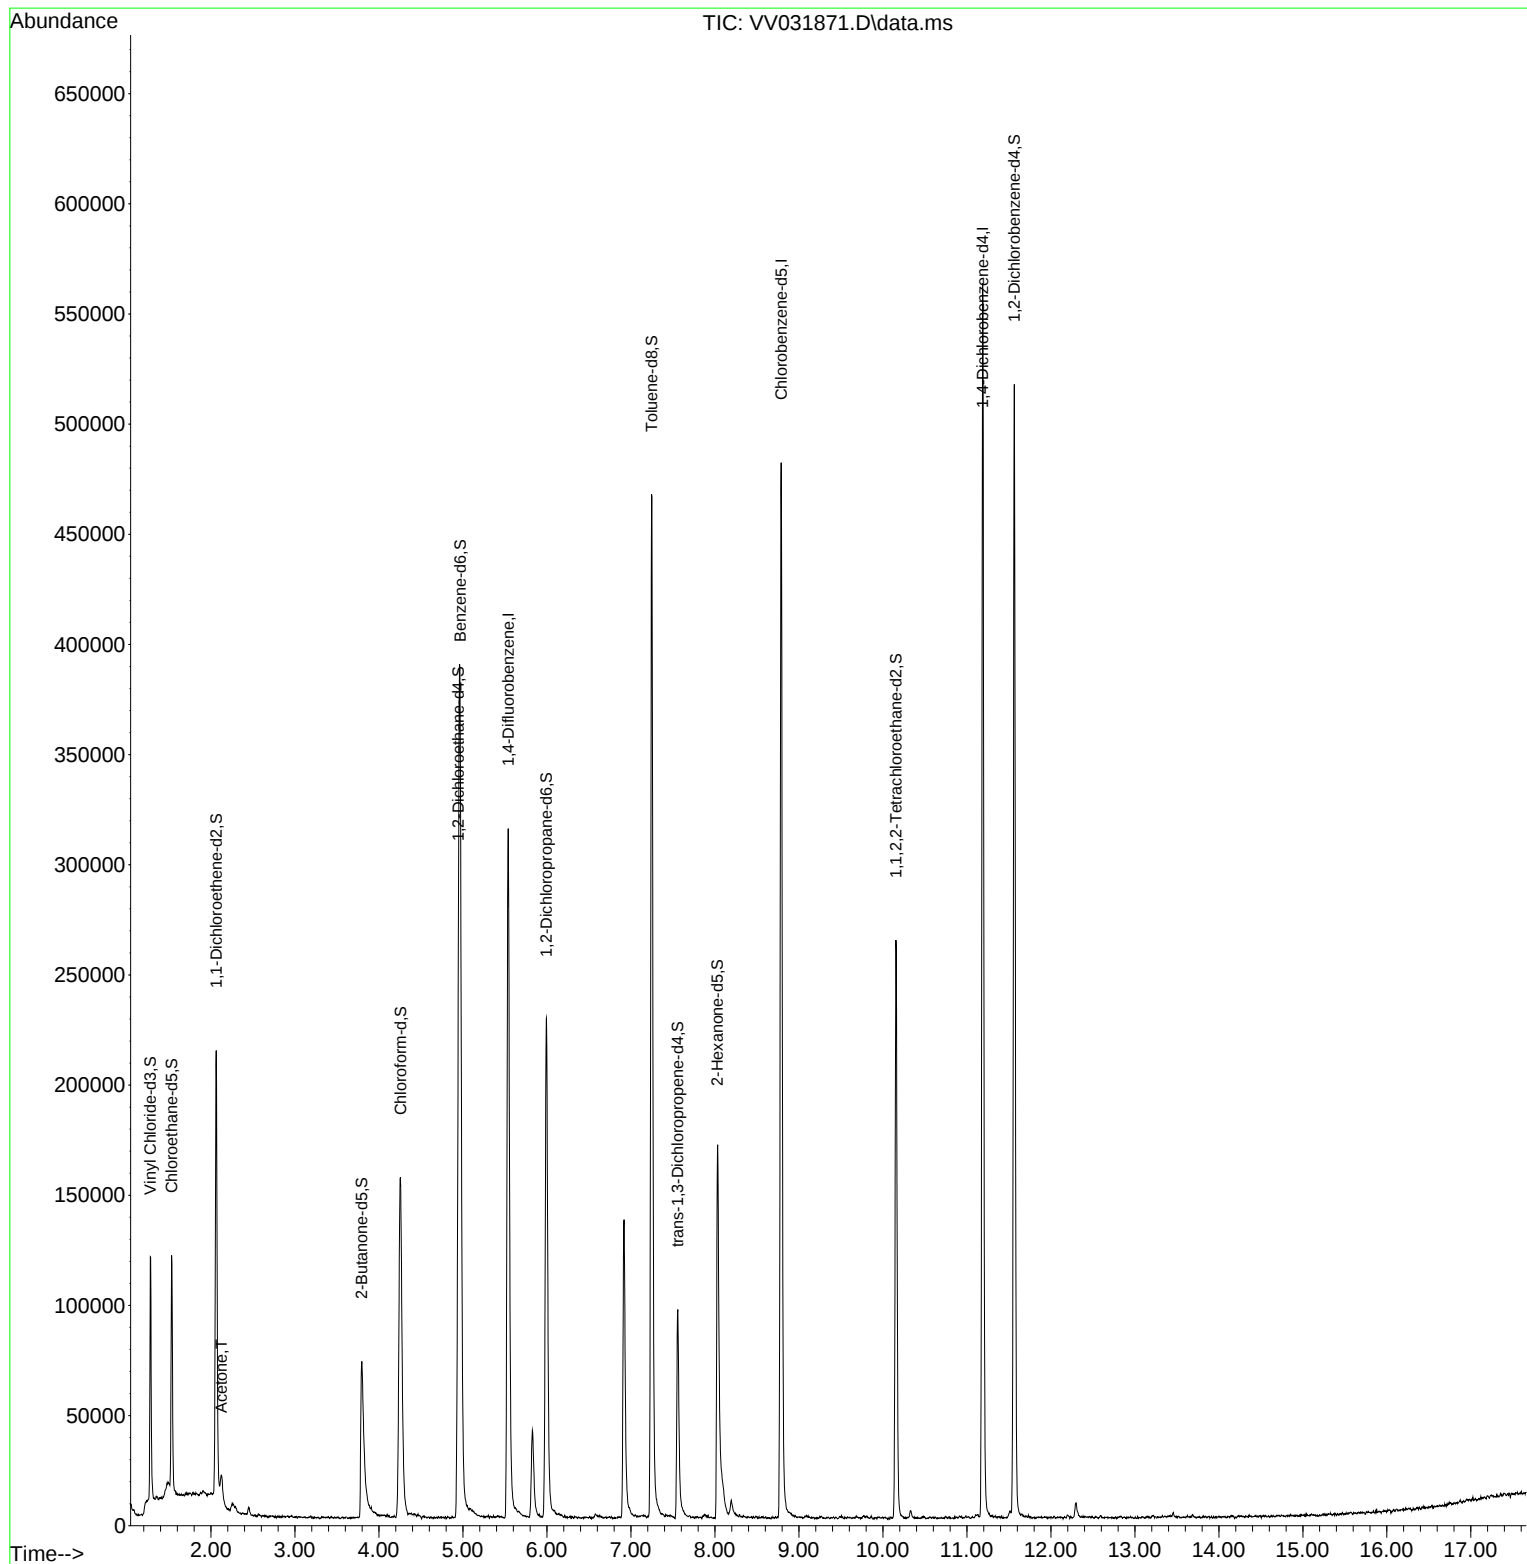

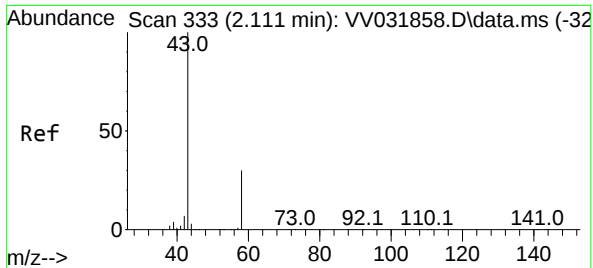

#13
 Acetone
 Concen: 6.614 ug/L
 RT: 2.124 min Scan# 31
 Delta R.T. 0.013 min
 Lab File: VV031871.D
 Acq: 23 Aug 2023 15:35

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN7

Tgt Ion: 43 Resp: 7728
 Ion Ratio Lower Upper
 43 100
 58 37.2 0.0 61.0

