

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW082323\  
 Data File : VW031872.D  
 Acq On : 23 Aug 2023 15:59  
 Operator : SY/MD  
 Sample : 04037-19  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EZYR2

Quant Time: Aug 24 01:58:22 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM082323WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Aug 24 01:40:47 2023  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc    | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|---------|--------|----------|
| -----                         |                |      |            |         |        |          |
| Internal Standards            |                |      |            |         |        |          |
| 1) 1,4-Difluorobenzene        | 5.538          | 114  | 266300     | 50.000  | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.789          | 117  | 258065     | 50.000  | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.191         | 152  | 135298     | 50.000  | ug/L   | 0.00     |
|                               |                |      |            |         |        |          |
| System Monitoring Compounds   |                |      |            |         |        |          |
| 4) Vinyl Chloride-d3          | 1.281          | 65   | 72970      | 43.784  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 135 |      | Recovery = | 87.560% |        |          |
| 7) Chloroethane-d5            | 1.532          | 69   | 66970      | 45.839  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 130 |      | Recovery = | 91.680% |        |          |
| 11) 1,1-Dichloroethene-d2     | 2.063          | 65   | 35021      | 44.876  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 89.760% |        |          |
| 21) 2-Butanone-d5             | 3.796          | 46   | 128882     | 98.325  | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 40 - 130 |      | Recovery = | 98.320% |        |          |
| 24) Chloroform-d              | 4.256          | 84   | 163906     | 44.995  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 90.000% |        |          |
| 26) 1,2-Dichloroethane-d4     | 4.947          | 65   | 112334     | 46.468  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 92.940% |        |          |
| 32) Benzene-d6                | 4.966          | 84   | 339528     | 48.216  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 96.440% |        |          |
| 36) 1,2-Dichloropropane-d6    | 5.992          | 67   | 109158     | 48.161  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 120 |      | Recovery = | 96.320% |        |          |
| 41) Toluene-d8                | 7.246          | 98   | 309967     | 47.773  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 95.540% |        |          |
| 43) trans-1,3-Dichloroprop... | 7.558          | 79   | 56063      | 47.723  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 95.440% |        |          |
| 47) 2-Hexanone-d5             | 8.030          | 63   | 60524      | 87.124  | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 45 - 130 |      | Recovery = | 87.120% |        |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.156         | 84   | 127316     | 43.469  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 120 |      | Recovery = | 86.940% |        |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.564         | 152  | 122884     | 49.823  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 99.640% |        |          |
|                               |                |      |            |         |        |          |
| Target Compounds              |                |      |            |         | Qvalue |          |
| 13) Acetone                   | 2.124          | 43   | 9442       | 8.093   | ug/L   | 94       |
| -----                         |                |      |            |         |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV082323\  
Data File : VV031872.D  
Acq On : 23 Aug 2023 15:59  
Operator : SY/MD  
Sample : 04037-19  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EZYR2

Quant Time: Aug 24 01:58:22 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM082323WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Aug 24 01:40:47 2023  
Response via : Initial Calibration

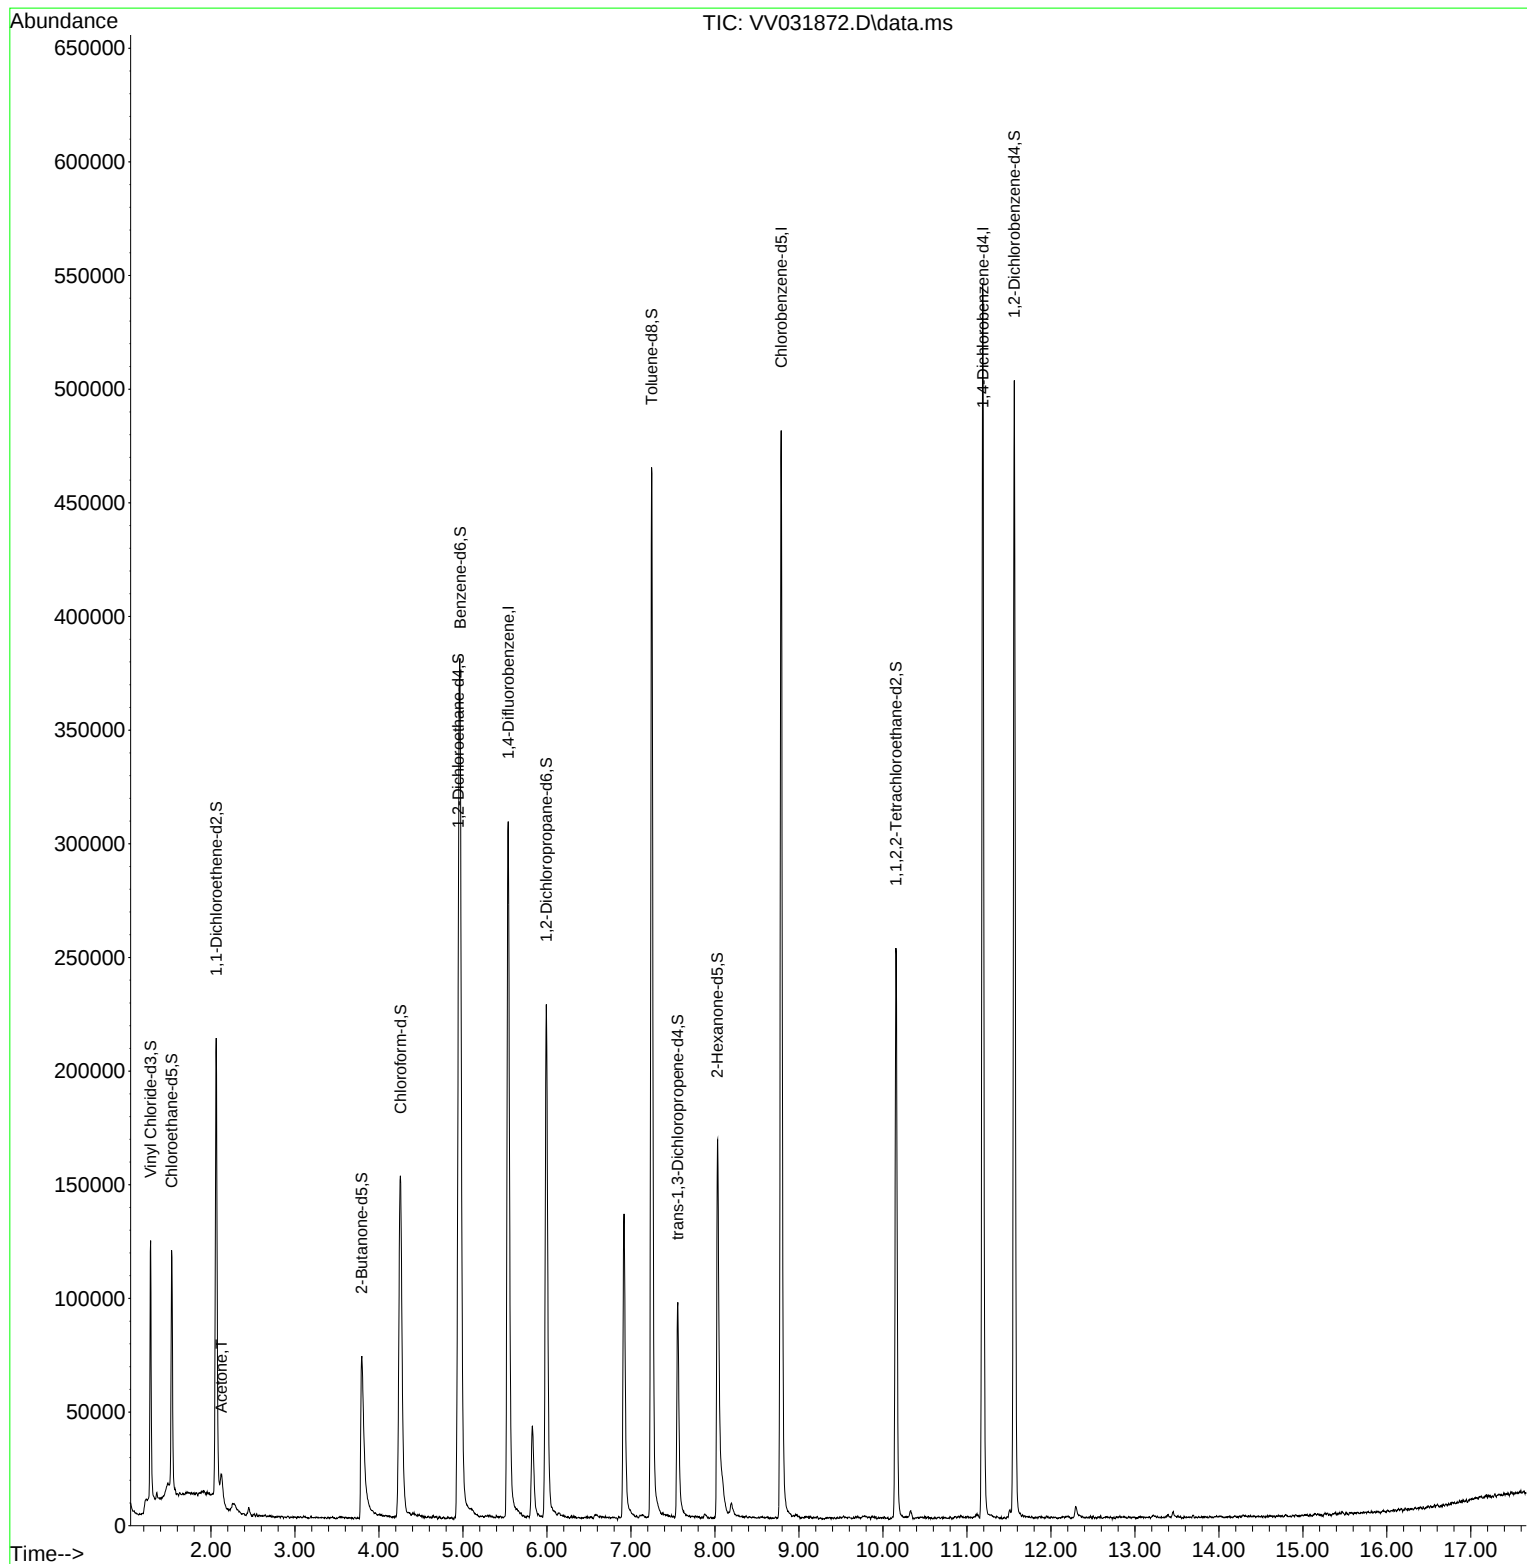

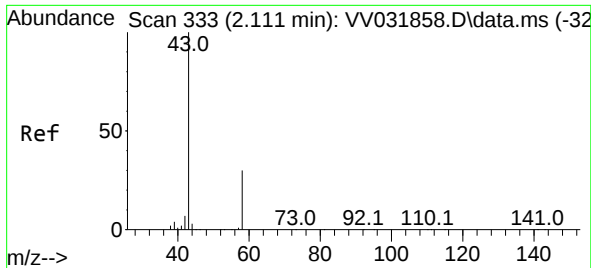

#13

Acetone

Concen: 8.093 ug/L

RT: 2.124 min Scan# 31

Delta R.T. 0.013 min

Lab File: VV031872.D

Acq: 23 Aug 2023 15:59

Instrument :

MSVOA\_V

ClientSampleId :

EZYR2

Tgt Ion: 43 Resp: 9442

Ion Ratio Lower Upper

43 100

58 33.9 0.0 61.0

