

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031862.D
 Acq On : 23 Aug 2023 12:09
 Operator : SY/MD
 Sample : VV0823MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK379

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	124910	130455	11.97%	1.494%
2	1.529	147	152	168	rVB	111001	131640	12.07%	1.508%
3	2.060	310	317	330	rVB	223475	318660	29.23%	3.650%
4	3.272	692	694	696	rBV3	628	354	0.03%	0.004%
5	3.285	696	698	700	rBV3	1092	623	0.06%	0.007%
6	3.548	777	780	782	rBV4	868	669	0.06%	0.008%
7	3.741	837	840	842	rBV4	870	544	0.05%	0.006%
8	3.786	845	854	883	rVV	85025	234552	21.51%	2.687%
9	4.249	984	998	1024	rBV	165336	419867	38.51%	4.809%
10	4.812	1169	1173	1174	rBV5	847	666	0.06%	0.008%
11	4.957	1202	1218	1242	rBV2	415060	1090282	100.00%	12.488%
12	5.487	1378	1383	1385	rBV6	1078	839	0.08%	0.010%
13	5.535	1386	1398	1420	rBV	335184	685014	62.83%	7.846%
14	5.825	1478	1488	1507	rBV2	29074	63311	5.81%	0.725%
15	5.989	1527	1539	1579	rBV	244271	510392	46.81%	5.846%
16	6.404	1666	1668	1669	rBV2	970	447	0.04%	0.005%
17	6.487	1692	1694	1699	rBV4	944	630	0.06%	0.007%
18	6.542	1709	1711	1714	rBV4	597	196	0.02%	0.002%
19	6.561	1714	1717	1719	rBV2	1458	1028	0.09%	0.012%
20	6.728	1765	1769	1771	rBV5	826	689	0.06%	0.008%
21	6.831	1798	1801	1806	rBV6	833	891	0.08%	0.010%
22	6.873	1812	1814	1815	rBV2	797	381	0.03%	0.004%
23	6.915	1816	1827	1852	rVV	149268	284836	26.12%	3.263%
24	7.246	1918	1930	1956	rBV	506363	903113	82.83%	10.344%
25	7.555	2016	2026	2049	rBV	105000	194183	17.81%	2.224%
26	7.908	2133	2136	2144	rVB7	2307	2883	0.26%	0.033%
27	7.969	2153	2155	2161	rBV5	648	626	0.06%	0.007%
28	8.027	2164	2173	2205	rBV	190109	379611	34.82%	4.348%
29	8.468	2308	2310	2315	rBV6	1016	721	0.07%	0.008%
30	8.529	2325	2329	2330	rBV4	807	637	0.06%	0.007%
31	8.786	2398	2409	2434	rBV	513009	869760	79.77%	9.962%
32	9.082	2496	2501	2502	rBV4	1824	1364	0.13%	0.016%
33	9.284	2562	2564	2569	rBV5	924	809	0.07%	0.009%
34	9.317	2572	2574	2576	rVB3	772	252	0.02%	0.003%
35	9.436	2607	2611	2614	rBV5	1001	755	0.07%	0.009%
36	9.583	2655	2657	2660	rVB3	979	525	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031862.D
 Acq On : 23 Aug 2023 12:09
 Operator : SY/MD
 Sample : VV0823MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK379

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	9.622	2664	2669	2671	rBV5	1549	1580	0.14%	0.018%
38	9.780	2715	2718	2719	rBV3	1054	739	0.07%	0.008%
39	9.831	2729	2734	2738	rBV7	1367	1737	0.16%	0.020%
40	9.908	2756	2758	2760	rVB3	607	229	0.02%	0.003%
41	9.998	2781	2786	2790	rBV5	1500	1268	0.12%	0.015%
42	10.108	2814	2820	2823	rBV7	1177	1155	0.11%	0.013%
43	10.156	2824	2835	2852	rVV	296733	476572	43.71%	5.459%
44	10.384	2902	2906	2912	rVB8	785	753	0.07%	0.009%
45	10.429	2918	2920	2924	rVB5	795	530	0.05%	0.006%
46	10.680	2996	2998	3002	rBV5	693	547	0.05%	0.006%
47	10.863	3044	3055	3064	rBV4	4439	8893	0.82%	0.102%
48	10.934	3073	3077	3080	rVB4	1115	1021	0.09%	0.012%
49	10.953	3080	3083	3085	rBV4	886	667	0.06%	0.008%
50	11.018	3099	3103	3107	rBV6	1178	1162	0.11%	0.013%
51	11.034	3107	3108	3109	rBV	454	150	0.01%	0.002%
52	11.133	3130	3139	3144	rBV7	4879	7765	0.71%	0.089%
53	11.188	3145	3156	3186	rVB	598578	946148	86.78%	10.837%
54	11.423	3226	3229	3231	rBV3	1084	872	0.08%	0.010%
55	11.471	3241	3244	3245	rBV3	686	353	0.03%	0.004%
56	11.522	3256	3260	3261	rBV4	595	458	0.04%	0.005%
57	11.564	3261	3273	3294	rVV	544359	866414	79.47%	9.924%
58	11.789	3340	3343	3349	rBV7	806	841	0.08%	0.010%
59	11.886	3371	3373	3375	rBV3	544	288	0.03%	0.003%
60	11.963	3395	3397	3400	rBV4	1194	727	0.07%	0.008%
61	12.111	3440	3443	3446	rBV5	1075	781	0.07%	0.009%
62	12.194	3467	3469	3471	rBV3	641	395	0.04%	0.005%
63	12.448	3544	3548	3554	rVB8	1238	1411	0.13%	0.016%
64	12.590	3583	3592	3600	rBV5	8191	14080	1.29%	0.161%
65	12.783	3650	3652	3658	rBV6	989	830	0.08%	0.010%
66	12.805	3658	3659	3660	rBV	631	189	0.02%	0.002%
67	12.860	3673	3676	3678	rVB4	838	439	0.04%	0.005%
68	12.976	3709	3712	3713	rBV2	544	307	0.03%	0.004%
69	13.005	3719	3721	3723	rBV3	483	211	0.02%	0.002%
70	13.017	3723	3725	3728	rBV3	840	667	0.06%	0.008%
71	13.114	3751	3755	3757	rBV5	1239	940	0.09%	0.011%
72	13.159	3768	3769	3771	rBV3	785	262	0.02%	0.003%
73	13.207	3775	3784	3796	rVB3	15570	24453	2.24%	0.280%
74	13.252	3796	3798	3799	rBV2	792	351	0.03%	0.004%
75	13.342	3823	3826	3828	rBV3	871	634	0.06%	0.007%
76	13.445	3849	3858	3873	rBV	60038	96144	8.82%	1.101%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031862.D
Acq On : 23 Aug 2023 12:09
Operator : SY/MD
Sample : VV0823MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis

77	13.686	3924	3933	3945	rBV	21320	35323	3.24%	0.405%
----	--------	------	------	------	-----	-------	-------	-------	--------




Sum of corrected areas: 8730491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031862.D
Acq On : 23 Aug 2023 12:09
Operator : SY/MD
Sample : VV0823MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

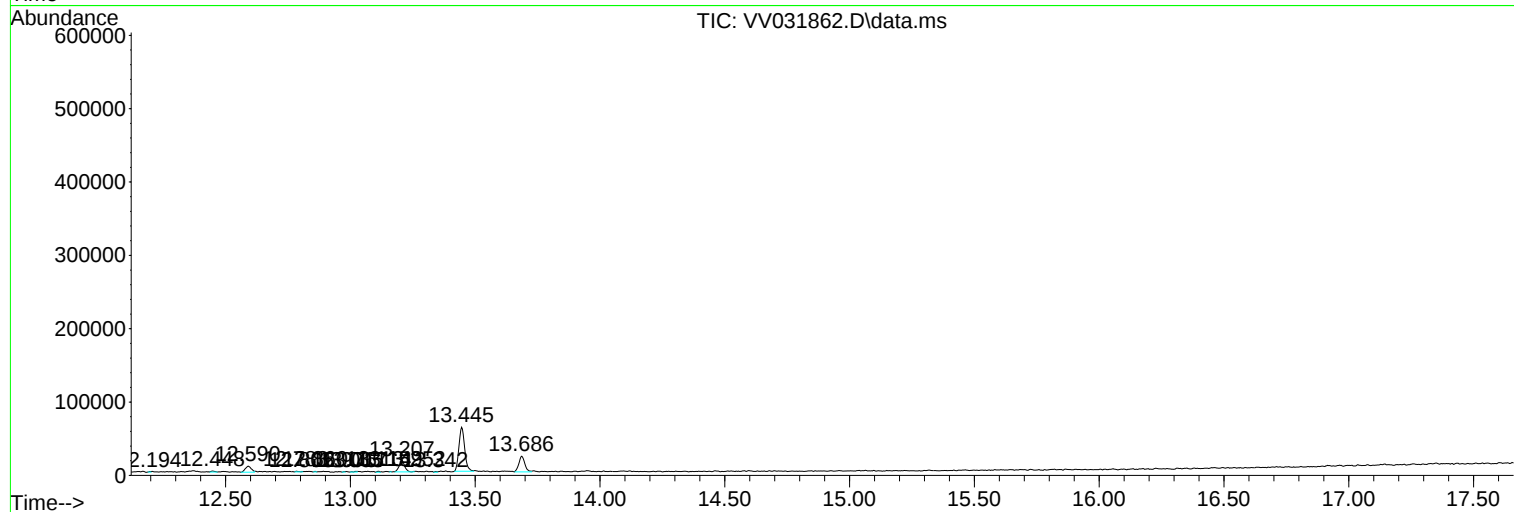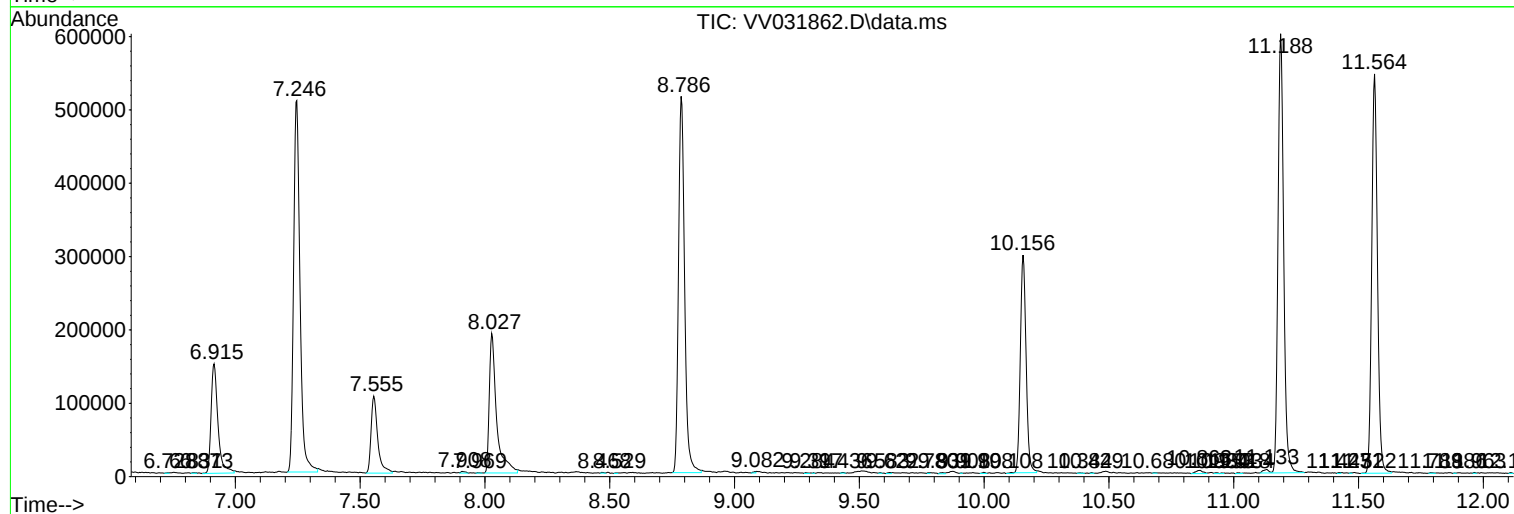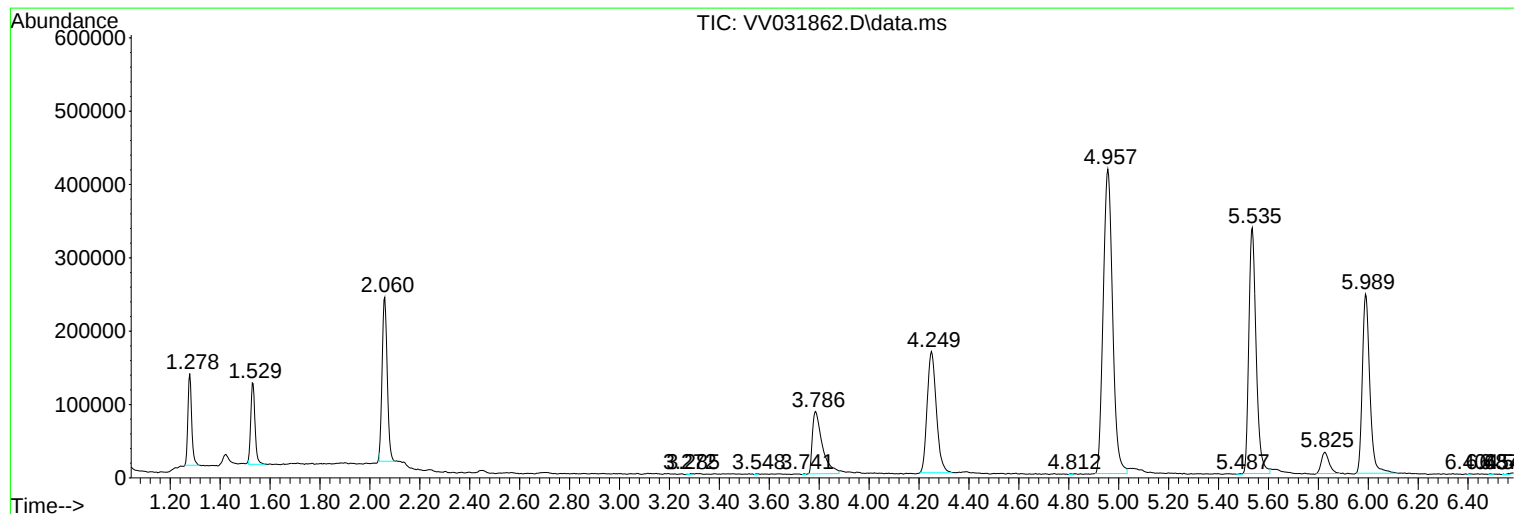

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031862.D
Acq On : 23 Aug 2023 12:09
Operator : SY/MD
Sample : VV0823MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031862.D
Acq On : 23 Aug 2023 12:09
Operator : SY/MD
Sample : VV0823MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc