

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031864.D
 Acq On : 23 Aug 2023 12:56
 Operator : SY/MD
 Sample : 04034-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	90	rVB	120906	127603	11.98%	1.537%
2	1.532	147	153	168	rVB	109006	130535	12.25%	1.572%
3	2.060	310	317	329	rVB	210175	293939	27.59%	3.539%
4	3.272	692	694	698	rBV3	563	346	0.03%	0.004%
5	3.378	725	727	728	rBV2	858	480	0.05%	0.006%
6	3.490	760	762	765	rBV3	855	450	0.04%	0.005%
7	3.571	783	787	788	rBV3	693	466	0.04%	0.006%
8	3.590	791	793	795	rBV2	778	433	0.04%	0.005%
9	3.651	810	812	816	rVB5	1177	776	0.07%	0.009%
10	3.680	819	821	822	rBV2	925	391	0.04%	0.005%
11	3.789	846	855	877	rBV	76713	200996	18.86%	2.420%
12	4.252	983	999	1023	rBV	161011	419070	39.33%	5.046%
13	4.664	1125	1127	1129	rBV3	705	350	0.03%	0.004%
14	4.715	1140	1143	1145	rBV4	712	559	0.05%	0.007%
15	4.873	1190	1192	1193	rVB2	339	96	0.01%	0.001%
16	4.886	1193	1196	1197	rBV3	443	241	0.02%	0.003%
17	4.960	1203	1219	1245	rBV2	402741	1065552	100.00%	12.831%
18	5.535	1386	1398	1422	rBV	329254	681511	63.96%	8.206%
19	5.825	1477	1488	1507	rBV	35566	78981	7.41%	0.951%
20	5.992	1528	1540	1564	rBV	232774	491238	46.10%	5.915%
21	6.362	1653	1655	1657	rBV3	771	408	0.04%	0.005%
22	6.448	1680	1682	1683	rBV2	494	222	0.02%	0.003%
23	6.500	1696	1698	1700	rBV3	416	242	0.02%	0.003%
24	6.545	1709	1712	1713	rBV3	500	354	0.03%	0.004%
25	6.571	1713	1720	1722	rBV7	1882	2280	0.21%	0.027%
26	6.706	1758	1762	1763	rBV3	749	560	0.05%	0.007%
27	6.799	1790	1791	1795	rBV4	606	374	0.04%	0.005%
28	6.860	1808	1810	1812	rBV3	848	442	0.04%	0.005%
29	6.915	1817	1827	1861	rVV	141833	277210	26.02%	3.338%
30	7.246	1919	1930	1965	rBV	480895	873081	81.94%	10.513%
31	7.554	2017	2026	2053	rBV	99918	184322	17.30%	2.220%
32	7.882	2121	2128	2138	rBV3	3727	6245	0.59%	0.075%
33	7.995	2161	2163	2164	rBV2	553	237	0.02%	0.003%
34	8.030	2165	2174	2207	rVV	175511	362553	34.02%	4.366%
35	8.481	2311	2314	2317	rBV5	700	545	0.05%	0.007%
36	8.542	2331	2333	2335	rBV3	487	275	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031864.D
 Acq On : 23 Aug 2023 12:56
 Operator : SY/MD
 Sample : 04034-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	8.696	2378	2381	2387	rVB7	902	626	0.06%	0.008%
38	8.722	2387	2389	2391	rBV2	828	477	0.04%	0.006%
39	8.789	2398	2410	2431	rBV	509226	851831	79.94%	10.257%
40	9.172	2526	2529	2533	rBV3	979	792	0.07%	0.010%
41	9.207	2536	2540	2543	rBV6	819	670	0.06%	0.008%
42	9.452	2610	2616	2617	rBV5	733	690	0.06%	0.008%
43	9.464	2617	2620	2622	rBV4	617	355	0.03%	0.004%
44	9.567	2650	2652	2656	rBV5	883	604	0.06%	0.007%
45	9.651	2674	2678	2682	rBV5	983	1040	0.10%	0.013%
46	9.841	2735	2737	2740	rBV3	804	376	0.04%	0.005%
47	9.870	2740	2746	2747	rBV3	1476	1451	0.14%	0.017%
48	9.972	2776	2778	2779	rBV2	507	245	0.02%	0.003%
49	10.008	2786	2789	2795	rBV8	1180	1357	0.13%	0.016%
50	10.062	2803	2806	2807	rBV2	746	469	0.04%	0.006%
51	10.075	2809	2810	2817	rVB7	1266	883	0.08%	0.011%
52	10.156	2825	2835	2859	rVB	283348	450474	42.28%	5.424%
53	10.255	2863	2866	2868	rBV4	806	539	0.05%	0.006%
54	10.384	2902	2906	2908	rBV4	674	458	0.04%	0.006%
55	10.542	2953	2955	2961	rVB4	1230	944	0.09%	0.011%
56	10.564	2961	2962	2963	rBV2	296	106	0.01%	0.001%
57	10.580	2963	2967	2970	rBV4	1316	1056	0.10%	0.013%
58	10.622	2977	2980	2981	rBV3	968	468	0.04%	0.006%
59	10.693	3000	3002	3003	rBV2	889	366	0.03%	0.004%
60	10.738	3014	3016	3017	rBV2	959	448	0.04%	0.005%
61	10.802	3034	3036	3039	rVB3	584	277	0.03%	0.003%
62	10.918	3068	3072	3078	rBV8	1270	1726	0.16%	0.021%
63	10.947	3079	3081	3084	rVV4	1026	544	0.05%	0.007%
64	11.075	3118	3121	3123	rBV3	1160	648	0.06%	0.008%
65	11.188	3145	3156	3180	rBV	580823	908370	85.25%	10.938%
66	11.390	3216	3219	3224	rBV5	875	803	0.08%	0.010%
67	11.490	3247	3250	3251	rBV3	730	432	0.04%	0.005%
68	11.516	3251	3258	3260	rVV6	2093	2665	0.25%	0.032%
69	11.564	3262	3273	3295	rVB	525369	823393	77.27%	9.915%
70	11.924	3382	3385	3387	rBV4	1001	556	0.05%	0.007%
71	11.940	3388	3390	3394	rBV5	601	520	0.05%	0.006%
72	12.297	3494	3501	3514	rBV7	6047	11639	1.09%	0.140%
73	12.445	3545	3547	3549	rBV3	956	492	0.05%	0.006%
74	12.512	3565	3568	3572	rBV5	736	641	0.06%	0.008%
75	12.545	3575	3578	3583	rVV6	1164	1228	0.12%	0.015%
76	12.586	3587	3591	3601	rVB10	3760	5732	0.54%	0.069%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031864.D
Acq On : 23 Aug 2023 12:56
Operator : SY/MD
Sample : 04034-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis

77	12.670	3612	3617	3621	rBV7	1465	1593	0.15%	0.019%
78	12.805	3655	3659	3660	rBV3	596	389	0.04%	0.005%
79	12.975	3711	3712	3715	rBV3	672	342	0.03%	0.004%
80	12.992	3715	3717	3719	rBV2	548	338	0.03%	0.004%
81	13.075	3740	3743	3744	rBV2	720	423	0.04%	0.005%
82	13.387	3835	3840	3844	rBV7	1632	1795	0.17%	0.022%
83	13.448	3851	3859	3873	rVB	10480	18531	1.74%	0.223%
84	13.619	3910	3912	3916	rBV5	1066	632	0.06%	0.008%
85	13.979	4021	4024	4025	rBV3	901	477	0.04%	0.006%
86	14.107	4063	4064	4065	rBV	733	277	0.03%	0.003%




Sum of corrected areas: 8304551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031864.D
Acq On : 23 Aug 2023 12:56
Operator : SY/MD
Sample : 04034-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

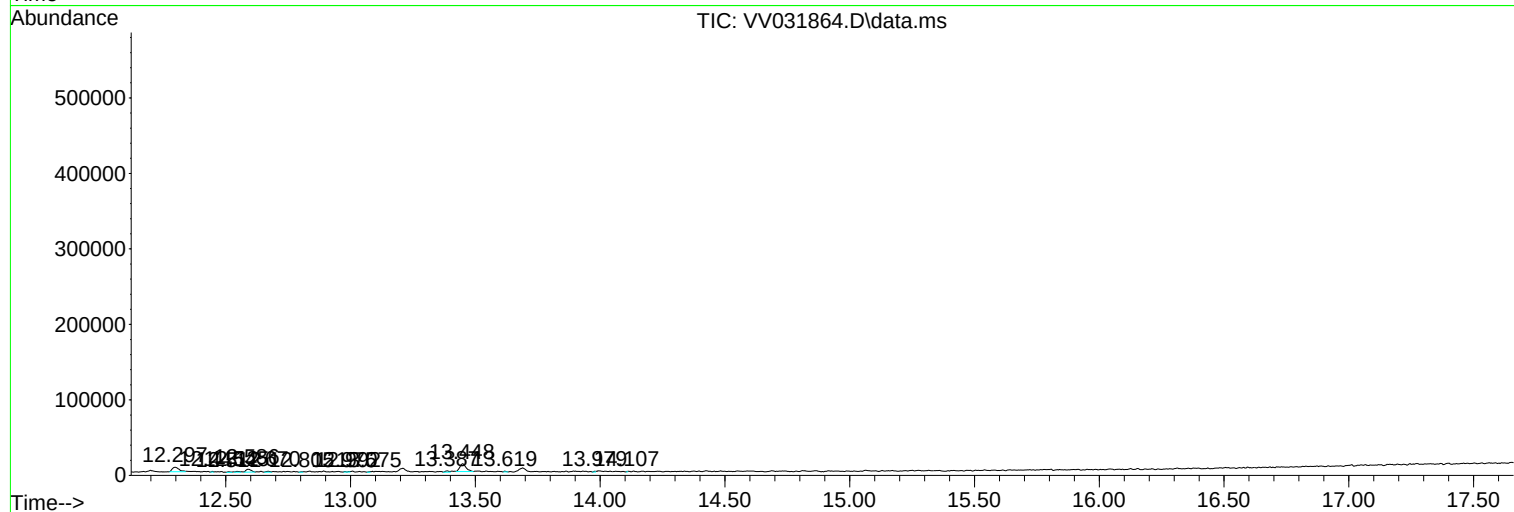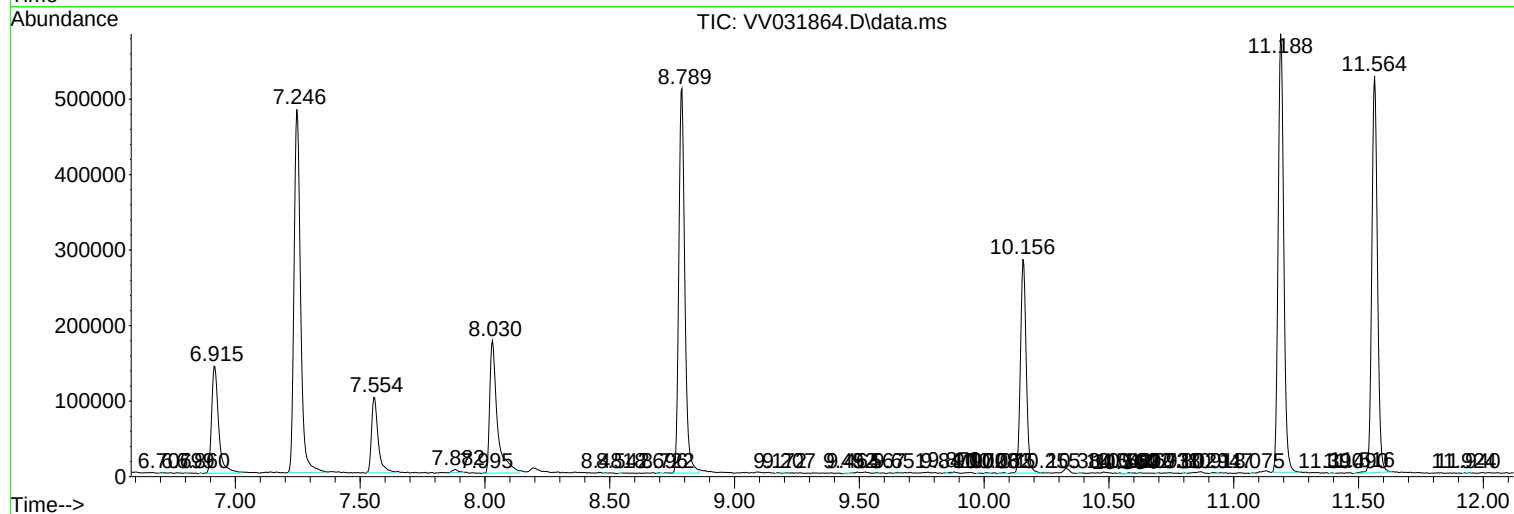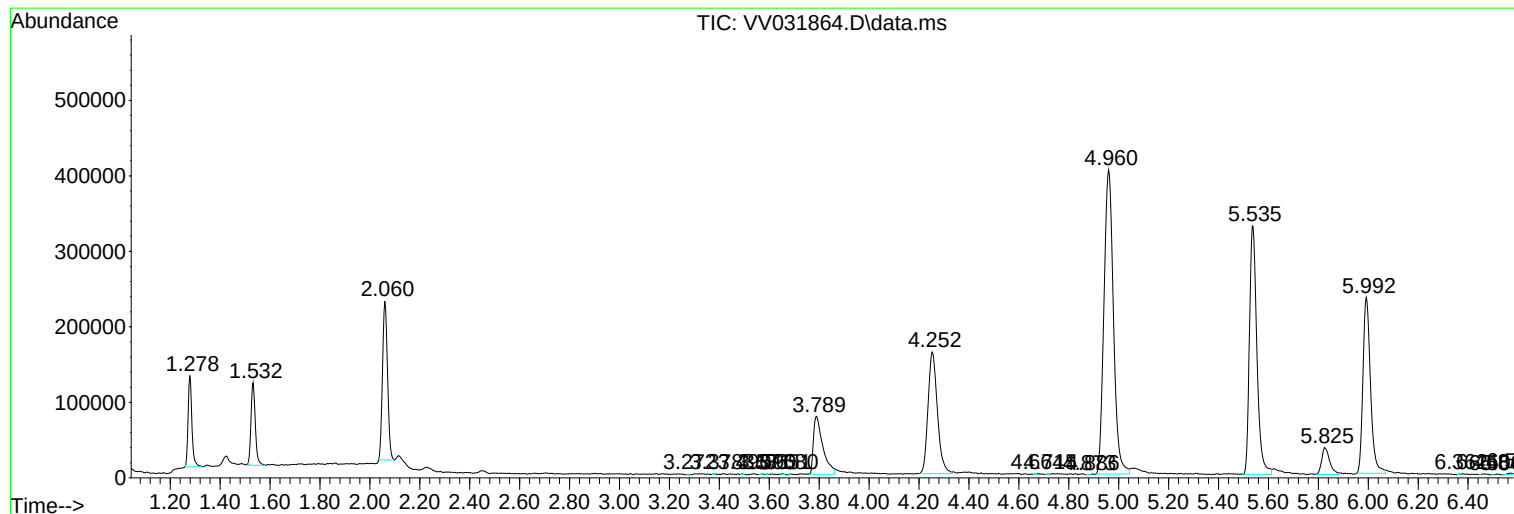

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031864.D
Acq On : 23 Aug 2023 12:56
Operator : SY/MD
Sample : 04034-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031864.D
Acq On : 23 Aug 2023 12:56
Operator : SY/MD
Sample : 04034-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYNS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc