

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031865.D
 Acq On : 23 Aug 2023 13:19
 Operator : SY/MD
 Sample : 04034-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	118143	125326	11.81%	1.517%
2	1.532	147	153	167	rVB	104827	124070	11.70%	1.502%
3	2.059	310	317	328	rVB	203865	284560	26.82%	3.445%
4	3.027	614	618	620	rBV3	829	720	0.07%	0.009%
5	3.101	639	641	643	rBV3	927	582	0.05%	0.007%
6	3.420	737	740	743	rBV4	1158	851	0.08%	0.010%
7	3.516	768	770	774	rVB5	993	501	0.05%	0.006%
8	3.555	780	782	785	rBV3	681	374	0.04%	0.005%
9	3.722	830	834	836	rBV5	684	430	0.04%	0.005%
10	3.789	845	855	884	rBV	80614	218086	20.56%	2.640%
11	4.143	961	965	966	rBV3	874	566	0.05%	0.007%
12	4.252	984	999	1022	rBV	158570	413162	38.95%	5.002%
13	4.574	1095	1099	1100	rBV4	1110	782	0.07%	0.009%
14	4.667	1125	1128	1131	rBV4	1152	908	0.09%	0.011%
15	4.702	1137	1139	1141	rVB3	859	393	0.04%	0.005%
16	4.731	1141	1148	1154	rBV10	934	1226	0.12%	0.015%
17	4.767	1156	1159	1160	rBV2	635	344	0.03%	0.004%
18	4.802	1167	1170	1173	rBV4	999	745	0.07%	0.009%
19	4.960	1202	1219	1244	rBV2	398069	1060878	100.00%	12.844%
20	5.448	1366	1371	1373	rBV7	1083	827	0.08%	0.010%
21	5.464	1373	1376	1379	rVV4	957	756	0.07%	0.009%
22	5.538	1387	1399	1427	rBV	316876	657284	61.96%	7.958%
23	5.828	1478	1489	1506	rBV2	37716	82740	7.80%	1.002%
24	5.992	1527	1540	1572	rBV	236836	502579	47.37%	6.085%
25	6.252	1618	1621	1624	rBV5	904	562	0.05%	0.007%
26	6.432	1675	1677	1679	rBV3	620	365	0.03%	0.004%
27	6.474	1687	1690	1691	rBV3	816	498	0.05%	0.006%
28	6.526	1699	1706	1711	rVB8	1046	1395	0.13%	0.017%
29	6.567	1716	1719	1720	rBV3	1397	862	0.08%	0.010%
30	6.802	1788	1792	1795	rBV6	966	892	0.08%	0.011%
31	6.828	1798	1800	1803	rVV4	739	344	0.03%	0.004%
32	6.863	1809	1811	1814	rVB3	768	356	0.03%	0.004%
33	6.918	1816	1828	1856	rBV	142906	276631	26.08%	3.349%
34	7.111	1885	1888	1890	rBV3	1302	917	0.09%	0.011%
35	7.246	1919	1930	1970	rBV	483625	876933	82.66%	10.617%
36	7.558	2017	2027	2054	rBV	98557	184188	17.36%	2.230%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031865.D
 Acq On : 23 Aug 2023 13:19
 Operator : SY/MD
 Sample : 04034-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.722	2075	2078	2079	rBV2	847	433	0.04%	0.005%
38	7.783	2096	2097	2101	rBV3	752	531	0.05%	0.006%
39	7.873	2119	2125	2126	rBV6	4114	3133	0.30%	0.038%
40	8.030	2165	2174	2206	rBV	183476	375899	35.43%	4.551%
41	8.410	2289	2292	2296	rBV5	999	1026	0.10%	0.012%
42	8.458	2305	2307	2313	rBV6	937	848	0.08%	0.010%
43	8.500	2318	2320	2325	rVB6	1470	990	0.09%	0.012%
44	8.619	2348	2357	2358	rBV8	1475	1376	0.13%	0.017%
45	8.731	2389	2392	2395	rBV4	1056	714	0.07%	0.009%
46	8.789	2399	2410	2433	rVV	496447	820344	77.33%	9.932%
47	9.143	2518	2520	2523	rVB4	1022	546	0.05%	0.007%
48	9.162	2523	2526	2528	rVB3	778	387	0.04%	0.005%
49	9.188	2528	2534	2535	rBV3	1270	1070	0.10%	0.013%
50	9.291	2564	2566	2570	rBV4	570	454	0.04%	0.005%
51	9.387	2593	2596	2598	rVB4	741	383	0.04%	0.005%
52	9.406	2598	2602	2606	rBV6	559	482	0.05%	0.006%
53	9.606	2663	2664	2669	rVB4	1015	697	0.07%	0.008%
54	9.641	2671	2675	2677	rBV5	913	656	0.06%	0.008%
55	9.988	2779	2783	2787	rBV4	795	768	0.07%	0.009%
56	10.030	2792	2796	2801	rVV6	597	679	0.06%	0.008%
57	10.078	2809	2811	2815	rVB4	612	437	0.04%	0.005%
58	10.156	2822	2835	2855	rBV	279569	453129	42.71%	5.486%
59	10.294	2875	2878	2881	rBV6	985	849	0.08%	0.010%
60	10.329	2881	2889	2899	rVB3	7744	12752	1.20%	0.154%
61	10.422	2913	2918	2921	rBV6	900	764	0.07%	0.009%
62	10.448	2923	2926	2928	rBV4	718	416	0.04%	0.005%
63	10.667	2990	2994	3000	rVB10	1054	1141	0.11%	0.014%
64	10.705	3003	3006	3007	rVB2	810	395	0.04%	0.005%
65	10.738	3011	3016	3022	rVB9	1041	1136	0.11%	0.014%
66	10.837	3044	3047	3049	rBV4	1144	773	0.07%	0.009%
67	10.956	3081	3084	3088	rBV5	854	728	0.07%	0.009%
68	11.082	3121	3123	3126	rBV4	793	416	0.04%	0.005%
69	11.101	3126	3129	3130	rBV2	1483	797	0.08%	0.010%
70	11.188	3145	3156	3177	rBV	568439	887530	83.66%	10.746%
71	11.516	3248	3258	3261	rBV9	3484	5432	0.51%	0.066%
72	11.564	3263	3273	3290	rVB	514042	816255	76.94%	9.883%
73	11.731	3323	3325	3326	rBV2	842	344	0.03%	0.004%
74	11.757	3330	3333	3336	rBV5	914	590	0.06%	0.007%
75	11.776	3336	3339	3341	rVB3	871	477	0.04%	0.006%
76	11.818	3348	3352	3357	rVB7	1040	753	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031865.D
 Acq On : 23 Aug 2023 13:19
 Operator : SY/MD
 Sample : 04034-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.850	3359	3362	3365	rBV3	871	711	0.07%	0.009%
78	11.901	3376	3378	3382	rVB4	652	406	0.04%	0.005%
79	12.104	3439	3441	3444	rBV4	961	517	0.05%	0.006%
80	12.201	3465	3471	3475	rBV3	2402	3291	0.31%	0.040%
81	12.297	3492	3501	3513	rBV7	5085	9997	0.94%	0.121%
82	12.429	3540	3542	3546	rBV4	864	558	0.05%	0.007%
83	12.641	3603	3608	3610	rBV5	953	990	0.09%	0.012%
84	12.673	3613	3618	3620	rBV6	1141	1027	0.10%	0.012%
85	12.818	3659	3663	3668	rBV7	1251	1325	0.12%	0.016%
86	12.975	3708	3712	3714	rBV3	708	527	0.05%	0.006%
87	13.011	3719	3723	3725	rBV6	1261	1032	0.10%	0.012%
88	13.120	3755	3757	3761	rBV4	636	430	0.04%	0.005%
89	13.207	3778	3784	3795	rVB4	3629	6207	0.59%	0.075%
90	13.287	3807	3809	3811	rBV3	781	451	0.04%	0.005%
91	13.397	3837	3843	3847	rBV7	1105	1621	0.15%	0.020%
92	13.590	3900	3903	3906	rVB4	821	436	0.04%	0.005%
93	13.638	3915	3918	3919	rBV2	757	357	0.03%	0.004%
94	13.689	3927	3934	3945	rBV7	4262	6881	0.65%	0.083%
95	13.844	3980	3982	3984	rBV3	790	374	0.04%	0.005%
96	14.069	4050	4052	4055	rBV4	1007	849	0.08%	0.010%
97	14.098	4059	4061	4063	rBV4	837	448	0.04%	0.005%
98	14.384	4148	4150	4152	rBV3	728	533	0.05%	0.006%
99	14.471	4175	4177	4183	rBV6	783	676	0.06%	0.008%
100	14.856	4295	4297	4302	rBV6	913	642	0.06%	0.008%




Sum of corrected areas: 8259449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031865.D
Acq On : 23 Aug 2023 13:19
Operator : SY/MD
Sample : 04034-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

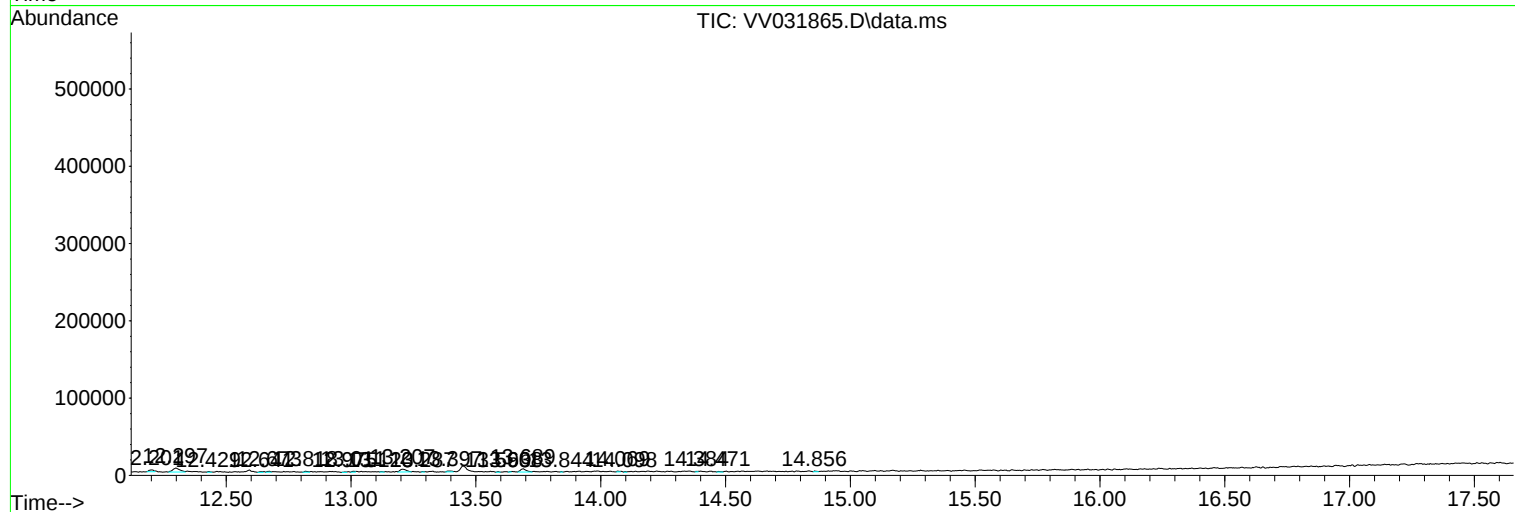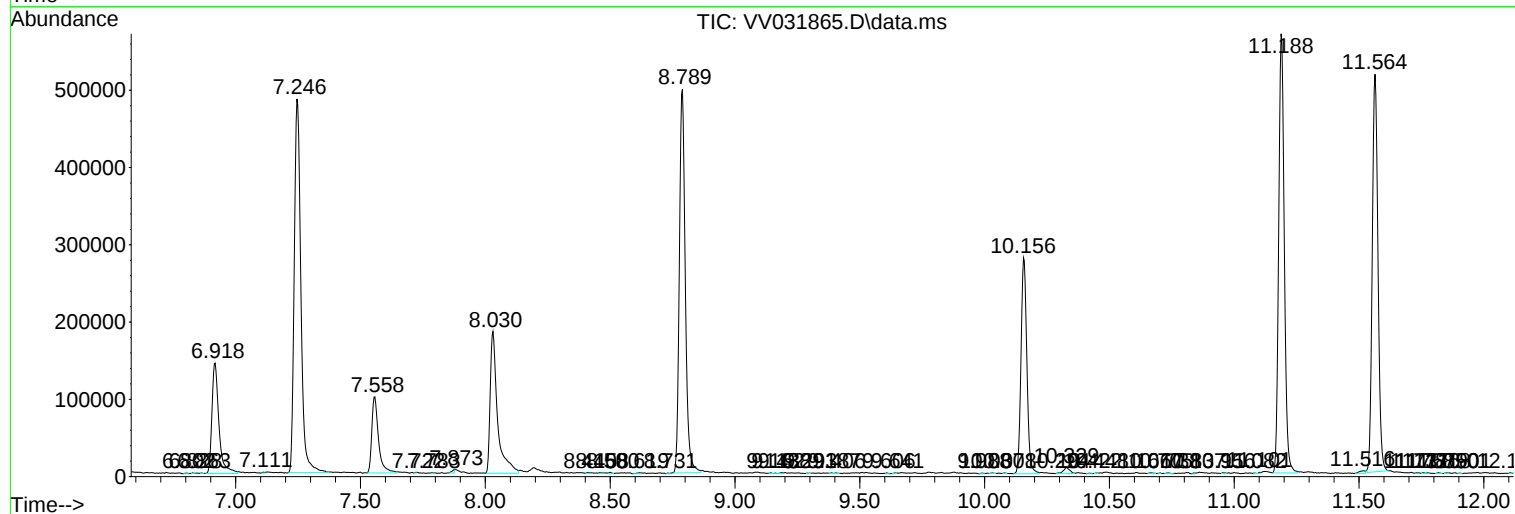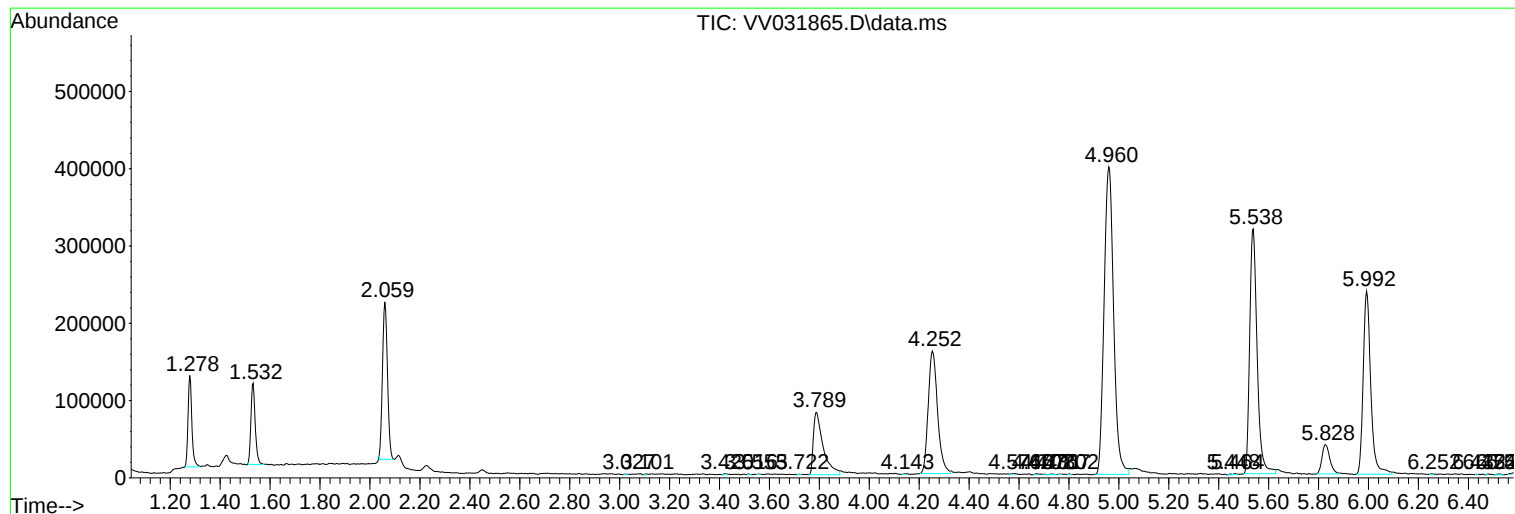

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031865.D
Acq On : 23 Aug 2023 13:19
Operator : SY/MD
Sample : 04034-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031865.D
Acq On : 23 Aug 2023 13:19
Operator : SY/MD
Sample : 04034-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc