

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031866.D
 Acq On : 23 Aug 2023 13:41
 Operator : SY/MD
 Sample : 04034-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	89	rVB	117698	123974	11.84%	1.459%
2	1.532	148	153	168	rVB	105887	124270	11.87%	1.462%
3	2.063	311	318	330	rVB	202254	286120	27.33%	3.367%
4	2.744	525	530	533	rBV5	1224	1169	0.11%	0.014%
5	3.114	643	645	651	rBV6	781	667	0.06%	0.008%
6	3.140	651	653	655	rBV4	728	284	0.03%	0.003%
7	3.400	731	734	739	rBV6	769	640	0.06%	0.008%
8	3.432	739	744	745	rBV5	965	916	0.09%	0.011%
9	3.625	796	804	810	rBV9	1239	2146	0.20%	0.025%
10	3.677	817	820	822	rBV2	1301	693	0.07%	0.008%
11	3.728	834	836	839	rBV3	626	503	0.05%	0.006%
12	3.789	845	855	882	rBV	76902	210556	20.11%	2.478%
13	4.259	984	1001	1035	rBV5	189787	647443	61.84%	7.619%
14	4.764	1156	1158	1161	rVB4	913	384	0.04%	0.005%
15	4.895	1196	1199	1201	rBV4	1075	797	0.08%	0.009%
16	4.963	1203	1220	1247	rVV2	394689	1046969	100.00%	12.320%
17	5.477	1378	1380	1383	rVB3	916	405	0.04%	0.005%
18	5.538	1387	1399	1419	rBV	315787	647775	61.87%	7.623%
19	5.828	1478	1489	1506	rBV2	30468	68451	6.54%	0.806%
20	5.992	1528	1540	1576	rBV	231799	487681	46.58%	5.739%
21	6.439	1669	1679	1695	rBV	45086	88392	8.44%	1.040%
22	6.561	1712	1717	1719	rBV5	1380	1393	0.13%	0.016%
23	6.812	1792	1795	1799	rBV4	739	689	0.07%	0.008%
24	6.918	1817	1828	1854	rBV	139625	270137	25.80%	3.179%
25	7.246	1919	1930	1962	rBV	477817	857233	81.88%	10.088%
26	7.558	2017	2027	2056	rBV	99455	189170	18.07%	2.226%
27	8.030	2163	2174	2205	rBV	179146	365245	34.89%	4.298%
28	8.352	2273	2274	2278	rVB2	727	338	0.03%	0.004%
29	8.532	2328	2330	2332	rBV3	674	309	0.03%	0.004%
30	8.574	2341	2343	2345	rBV2	594	324	0.03%	0.004%
31	8.606	2351	2353	2354	rBV2	518	187	0.02%	0.002%
32	8.718	2386	2388	2390	rBV3	560	247	0.02%	0.003%
33	8.789	2397	2410	2432	rBV	492105	834528	79.71%	9.821%
34	9.021	2480	2482	2487	rBV5	608	553	0.05%	0.007%
35	9.136	2515	2518	2521	rVB4	661	425	0.04%	0.005%
36	9.156	2521	2524	2525	rBV3	719	377	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW082323\
 Data File : VW031866.D
 Acq On : 23 Aug 2023 13:41
 Operator : SY/MD
 Sample : 04034-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	9.307	2568	2571	2573	rBV4	687	459	0.04%	0.005%
38	9.381	2587	2594	2595	rBV6	739	864	0.08%	0.010%
39	9.558	2644	2649	2653	rBV6	1034	960	0.09%	0.011%
40	9.583	2653	2657	2661	rBV5	924	775	0.07%	0.009%
41	9.628	2669	2671	2675	rVB4	755	365	0.03%	0.004%
42	9.670	2675	2684	2692	rBV10	2716	5062	0.48%	0.060%
43	9.998	2783	2786	2787	rBV3	697	343	0.03%	0.004%
44	10.040	2796	2799	2802	rBV5	939	575	0.05%	0.007%
45	10.098	2816	2817	2819	rBV2	453	161	0.02%	0.002%
46	10.156	2824	2835	2853	rVV	287990	462437	44.17%	5.442%
47	10.291	2875	2877	2880	rVB3	1539	614	0.06%	0.007%
48	10.329	2880	2889	2900	rBV2	8624	14795	1.41%	0.174%
49	10.381	2900	2905	2908	rBV5	658	648	0.06%	0.008%
50	10.423	2916	2918	2921	rBV3	689	445	0.04%	0.005%
51	10.487	2934	2938	2942	rBV5	971	1039	0.10%	0.012%
52	10.609	2975	2976	2979	rBV3	593	249	0.02%	0.003%
53	10.625	2979	2981	2982	rBV2	793	338	0.03%	0.004%
54	10.808	3035	3038	3040	rBV3	1449	919	0.09%	0.011%
55	10.905	3065	3068	3069	rBV3	616	271	0.03%	0.003%
56	10.927	3073	3075	3077	rBV2	633	271	0.03%	0.003%
57	11.053	3109	3114	3117	rBV6	822	702	0.07%	0.008%
58	11.085	3122	3124	3125	rBV	655	308	0.03%	0.004%
59	11.127	3132	3137	3139	rBV5	1772	1692	0.16%	0.020%
60	11.188	3145	3156	3178	rBV	575094	906571	86.59%	10.668%
61	11.467	3239	3243	3245	rBV4	1179	726	0.07%	0.009%
62	11.564	3261	3273	3300	rBV	518911	824361	78.74%	9.701%
63	11.754	3331	3332	3333	rBV2	407	124	0.01%	0.001%
64	11.783	3339	3341	3343	rBV3	469	269	0.03%	0.003%
65	11.885	3370	3373	3376	rVB4	1437	826	0.08%	0.010%
66	12.001	3407	3409	3413	rVB4	687	266	0.03%	0.003%
67	12.139	3448	3452	3454	rBV3	656	472	0.05%	0.006%
68	12.156	3454	3457	3460	rBV4	613	457	0.04%	0.005%
69	12.394	3527	3531	3534	rBV5	1153	957	0.09%	0.011%
70	12.593	3587	3593	3599	rBV8	1780	2405	0.23%	0.028%
71	12.757	3641	3644	3646	rBV3	1163	827	0.08%	0.010%
72	12.876	3676	3681	3683	rBV5	1166	1133	0.11%	0.013%
73	13.024	3724	3727	3729	rBV4	672	469	0.04%	0.006%
74	13.522	3879	3882	3885	rBV5	867	637	0.06%	0.007%
75	13.744	3947	3951	3954	rBV5	830	737	0.07%	0.009%
76	13.805	3968	3970	3973	rBV3	805	496	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031866.D
Acq On : 23 Aug 2023 13:41
Operator : SY/MD
Sample : 04034-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis

77	13.847	3980	3983	3986	rBV2	707	392	0.04%	0.005%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 8497807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031866.D
Acq On : 23 Aug 2023 13:41
Operator : SY/MD
Sample : 04034-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

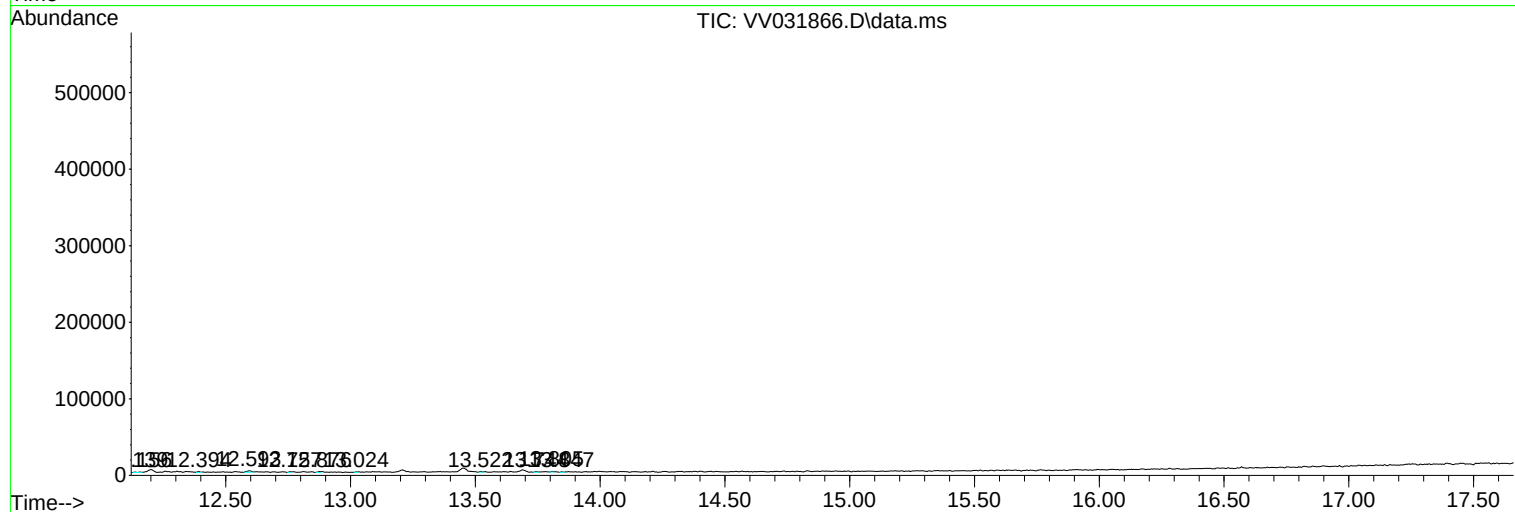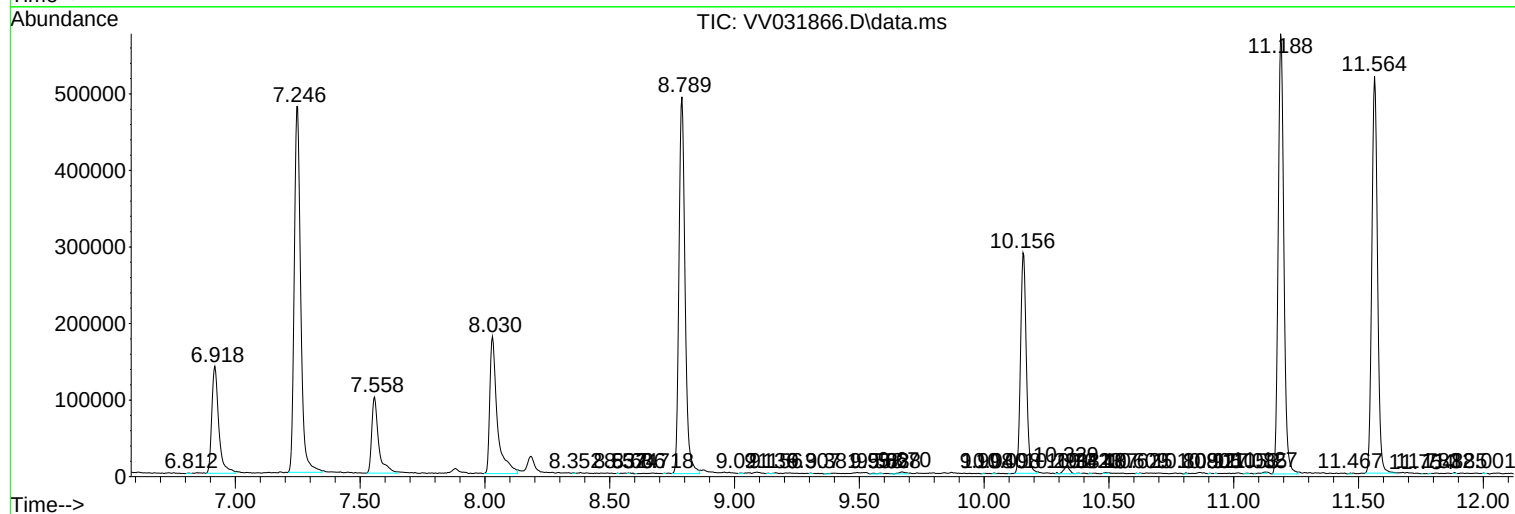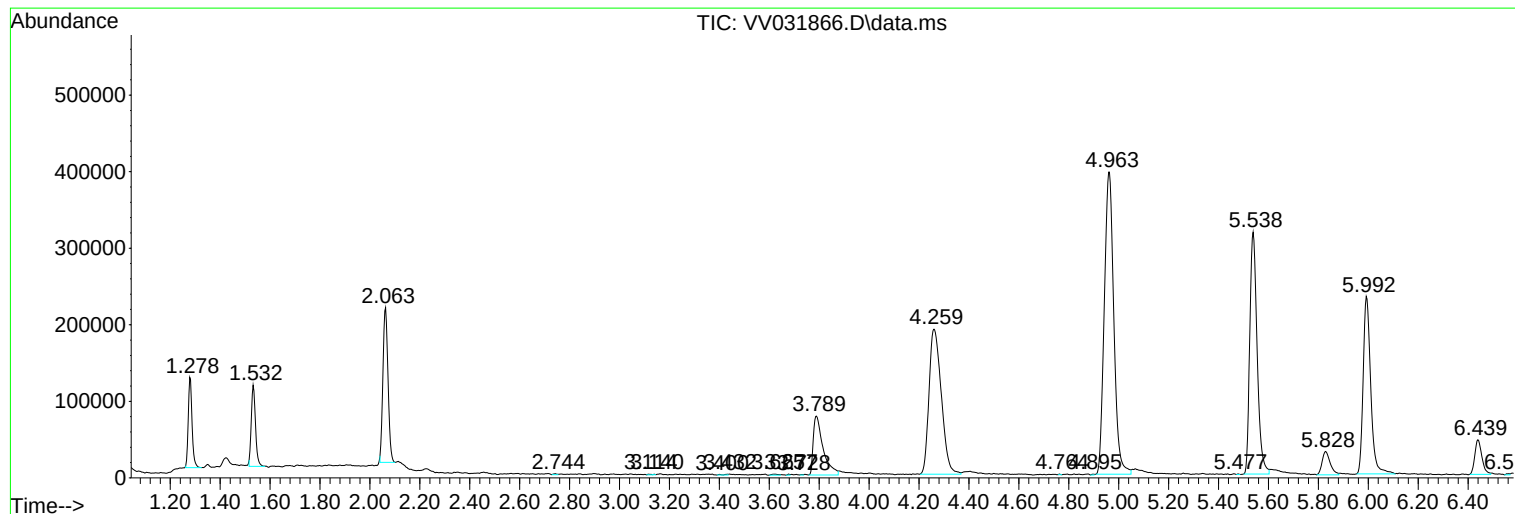

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031866.D
Acq On : 23 Aug 2023 13:41
Operator : SY/MD
Sample : 04034-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031866.D
Acq On : 23 Aug 2023 13:41
Operator : SY/MD
Sample : 04034-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc