

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031867.D
 Acq On : 23 Aug 2023 14:03
 Operator : SY/MD
 Sample : 04034-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	116847	122534	11.47%	1.475%
2	1.532	147	153	166	rVB	113605	126909	11.88%	1.528%
3	2.060	310	317	329	rVB	203654	285665	26.74%	3.439%
4	2.626	490	493	496	rBV4	1040	882	0.08%	0.011%
5	2.774	536	539	540	rBV2	693	490	0.05%	0.006%
6	2.889	566	575	576	rBV8	1266	1363	0.13%	0.016%
7	3.130	647	650	655	rVB5	761	702	0.07%	0.008%
8	3.339	713	715	718	rBV4	639	485	0.05%	0.006%
9	3.426	739	742	746	rVB5	898	700	0.07%	0.008%
10	3.462	751	753	755	rBV2	619	421	0.04%	0.005%
11	3.536	774	776	779	rVB3	875	412	0.04%	0.005%
12	3.632	800	806	808	rBV5	919	792	0.07%	0.010%
13	3.790	846	855	890	rBV	75066	211625	19.81%	2.548%
14	4.253	986	999	1028	rVB	159275	406146	38.01%	4.890%
15	4.619	1108	1113	1119	rVB8	1259	1276	0.12%	0.015%
16	4.648	1119	1122	1126	rBV7	731	566	0.05%	0.007%
17	4.687	1130	1134	1138	rBV7	846	943	0.09%	0.011%
18	4.745	1148	1152	1155	rBV4	1481	1123	0.11%	0.014%
19	4.838	1178	1181	1183	rBV4	668	349	0.03%	0.004%
20	4.860	1186	1188	1196	rVB7	701	627	0.06%	0.008%
21	4.896	1196	1199	1202	rBV4	913	602	0.06%	0.007%
22	4.960	1202	1219	1243	rBV2	405816	1068398	100.00%	12.863%
23	5.394	1351	1354	1356	rBV4	909	642	0.06%	0.008%
24	5.539	1387	1399	1423	rBV	319640	661055	61.87%	7.959%
25	5.828	1478	1489	1506	rBV3	38126	82024	7.68%	0.988%
26	5.992	1527	1540	1576	rBV	235727	503472	47.12%	6.061%
27	6.227	1611	1613	1615	rVB3	1002	405	0.04%	0.005%
28	6.362	1653	1655	1660	rVV5	560	436	0.04%	0.005%
29	6.416	1668	1672	1675	rBV6	1161	929	0.09%	0.011%
30	6.780	1784	1785	1790	rVB4	882	528	0.05%	0.006%
31	6.841	1801	1804	1807	rBV5	610	560	0.05%	0.007%
32	6.918	1817	1828	1856	rBV	142534	274662	25.71%	3.307%
33	7.246	1919	1930	1968	rBV	480847	872212	81.64%	10.501%
34	7.558	2018	2027	2046	rBV	99835	180530	16.90%	2.173%
35	7.883	2114	2128	2136	rBV4	6818	13634	1.28%	0.164%
36	7.944	2143	2147	2152	rVB6	746	717	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031867.D
 Acq On : 23 Aug 2023 14:03
 Operator : SY/MD
 Sample : 04034-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.966	2152	2154	2157	rBV4	800	663	0.06%	0.008%
38	8.031	2165	2174	2211	rBV	178051	367511	34.40%	4.425%
39	8.355	2271	2275	2277	rBV4	1374	1004	0.09%	0.012%
40	8.432	2297	2299	2302	rBV4	1122	644	0.06%	0.008%
41	8.487	2313	2316	2320	rBV5	727	584	0.05%	0.007%
42	8.577	2340	2344	2346	rBV4	569	414	0.04%	0.005%
43	8.635	2358	2362	2367	rBV7	1222	1338	0.13%	0.016%
44	8.789	2398	2410	2439	rBV	495272	838872	78.52%	10.099%
45	9.133	2513	2517	2523	rVB8	1099	1052	0.10%	0.013%
46	9.262	2554	2557	2560	rBV4	822	706	0.07%	0.008%
47	9.294	2564	2567	2569	rBV4	500	358	0.03%	0.004%
48	9.522	2633	2638	2644	rBV6	853	1209	0.11%	0.015%
49	9.690	2687	2690	2695	rBV6	1160	991	0.09%	0.012%
50	9.715	2695	2698	2699	rBV3	745	464	0.04%	0.006%
51	9.860	2738	2743	2745	rBV5	865	960	0.09%	0.012%
52	9.908	2756	2758	2765	rVB7	658	389	0.04%	0.005%
53	10.053	2802	2803	2808	rVB5	653	372	0.03%	0.004%
54	10.092	2811	2815	2818	rVB5	1027	771	0.07%	0.009%
55	10.156	2820	2835	2859	rBV	275016	448293	41.96%	5.397%
56	10.330	2878	2889	2899	rVV2	13630	23063	2.16%	0.278%
57	10.420	2913	2917	2918	rBV2	713	472	0.04%	0.006%
58	10.458	2926	2929	2932	rBV4	543	463	0.04%	0.006%
59	10.619	2977	2979	2983	rBV5	709	435	0.04%	0.005%
60	10.735	3010	3015	3018	rBV7	735	589	0.06%	0.007%
61	10.760	3021	3023	3026	rVV4	588	371	0.03%	0.004%
62	10.783	3026	3030	3035	rVV6	831	546	0.05%	0.007%
63	10.802	3035	3036	3041	rBV4	520	383	0.04%	0.005%
64	10.969	3086	3088	3091	rVB5	1295	800	0.07%	0.010%
65	10.992	3091	3095	3100	rVB7	644	458	0.04%	0.006%
66	11.021	3100	3104	3107	rBV5	1045	732	0.07%	0.009%
67	11.127	3125	3137	3145	rBV5	2059	4726	0.44%	0.057%
68	11.188	3145	3156	3176	rBV	595776	903987	84.61%	10.883%
69	11.448	3235	3237	3244	rVB6	1136	1132	0.11%	0.014%
70	11.481	3244	3247	3248	rBV3	716	410	0.04%	0.005%
71	11.519	3251	3259	3261	rVV5	2596	3879	0.36%	0.047%
72	11.564	3262	3273	3295	rVB	528475	839894	78.61%	10.112%
73	11.760	3332	3334	3337	rBV3	711	574	0.05%	0.007%
74	11.857	3361	3364	3367	rVB5	656	358	0.03%	0.004%
75	11.902	3375	3378	3380	rBV4	737	538	0.05%	0.006%
76	11.956	3391	3395	3399	rBV6	1280	1287	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031867.D
 Acq On : 23 Aug 2023 14:03
 Operator : SY/MD
 Sample : 04034-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	12.072	3428	3431	3435	rVB5	598	447	0.04%	0.005%
78	12.169	3459	3461	3462	rBV2	992	418	0.04%	0.005%
79	12.297	3494	3501	3507	rBV6	5569	8235	0.77%	0.099%
80	12.458	3548	3551	3556	rBV7	805	612	0.06%	0.007%
81	12.555	3578	3581	3582	rBV3	984	424	0.04%	0.005%
82	12.590	3588	3592	3598	rVB7	1399	1531	0.14%	0.018%
83	12.825	3663	3665	3668	rVB4	863	447	0.04%	0.005%
84	12.931	3695	3698	3700	rBV3	675	426	0.04%	0.005%
85	12.966	3706	3709	3713	rBV3	823	575	0.05%	0.007%
86	12.989	3713	3716	3721	rVB4	980	812	0.08%	0.010%
87	13.059	3734	3738	3741	rBV5	791	711	0.07%	0.009%
88	13.124	3755	3758	3759	rBV3	849	427	0.04%	0.005%
89	13.204	3779	3783	3787	rBV5	2668	2717	0.25%	0.033%
90	13.294	3808	3811	3815	rBV6	917	884	0.08%	0.011%
91	13.378	3834	3837	3838	rBV2	743	432	0.04%	0.005%
92	13.448	3854	3859	3860	rBV5	3258	2867	0.27%	0.035%
93	13.538	3883	3887	3890	rVB5	1247	969	0.09%	0.012%
94	13.567	3890	3896	3897	rBV5	863	662	0.06%	0.008%
95	13.590	3901	3903	3906	rBV5	629	402	0.04%	0.005%
96	13.686	3929	3933	3941	rBV8	2469	3363	0.31%	0.040%
97	13.741	3946	3950	3952	rBV4	794	642	0.06%	0.008%
98	14.243	4103	4106	4109	rBV4	960	601	0.06%	0.007%
99	14.320	4127	4130	4131	rBV3	746	432	0.04%	0.005%
100	14.844	4291	4293	4296	rBV3	1019	541	0.05%	0.007%




Sum of corrected areas: 8306085

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031867.D
Acq On : 23 Aug 2023 14:03
Operator : SY/MD
Sample : 04034-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

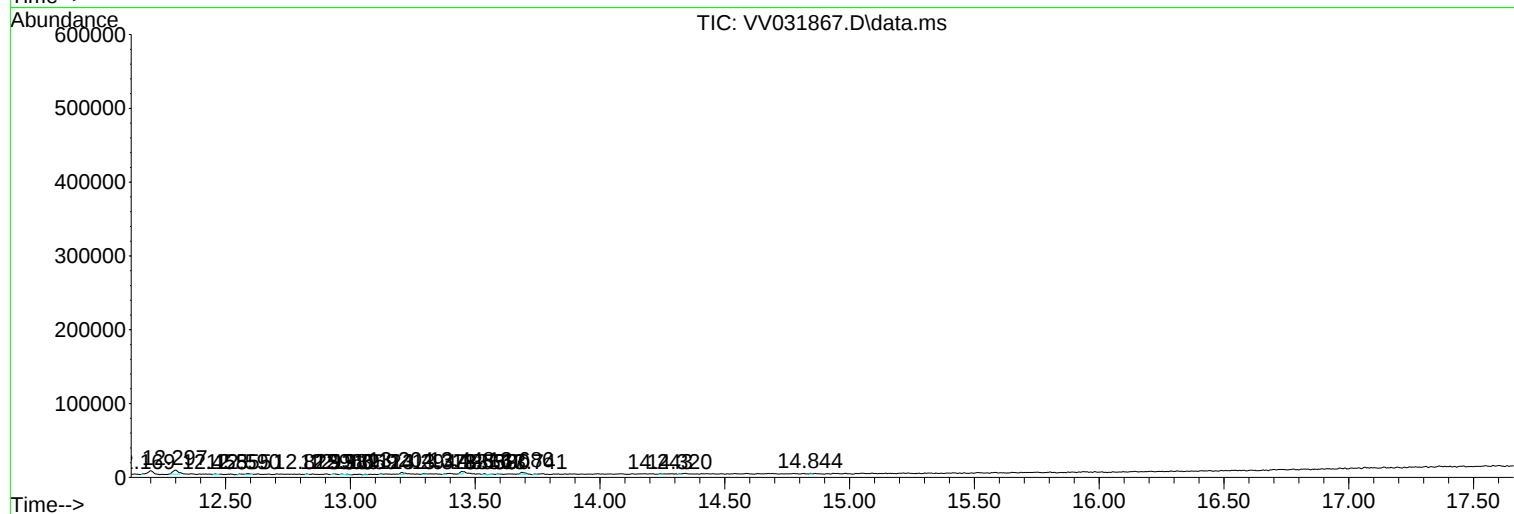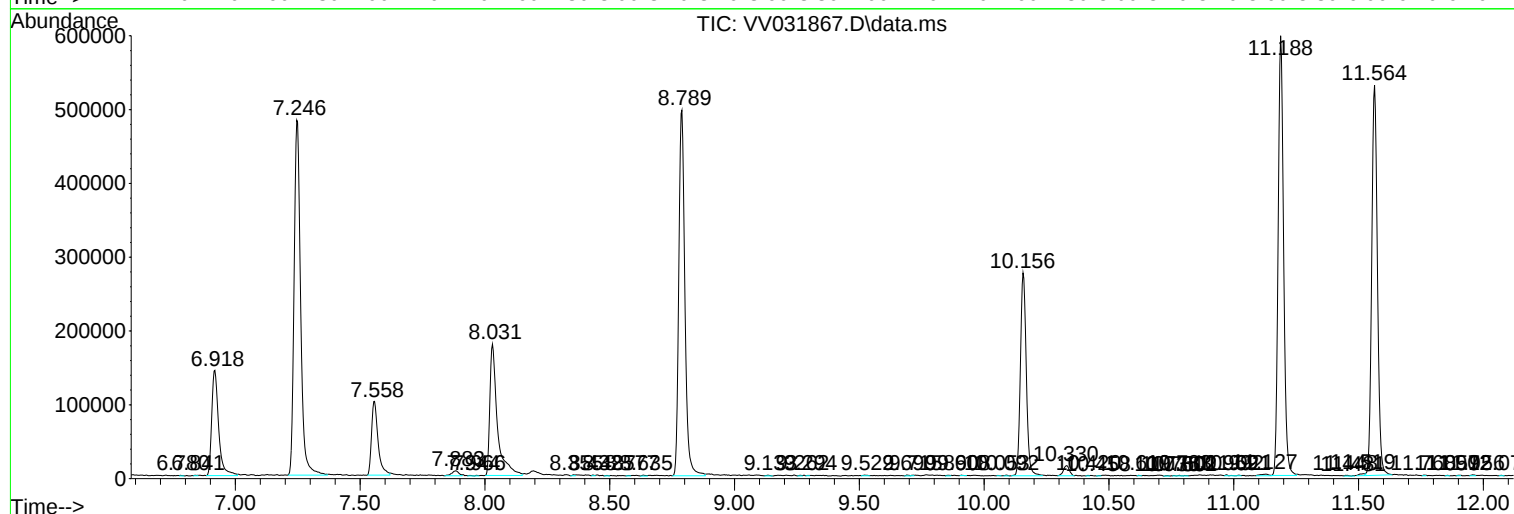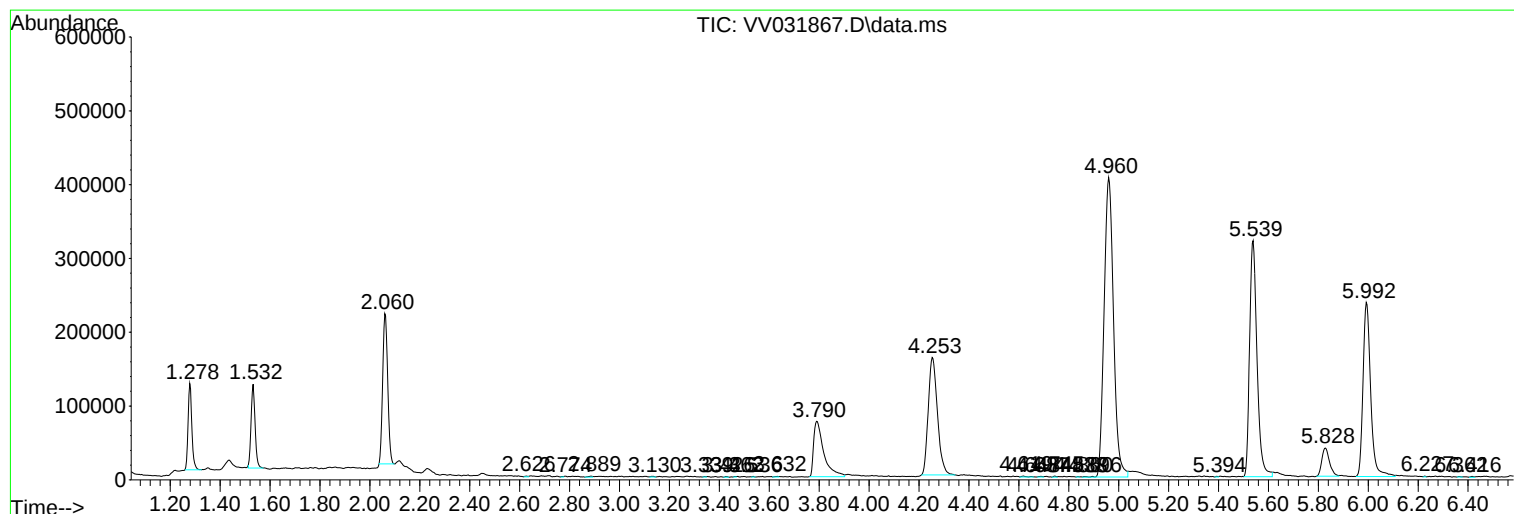

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031867.D
Acq On : 23 Aug 2023 14:03
Operator : SY/MD
Sample : 04034-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYNG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031867.D
Acq On : 23 Aug 2023 14:03
Operator : SY/MD
Sample : 04034-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYNG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc