

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031868.D
 Acq On : 23 Aug 2023 14:27
 Operator : SY/MD
 Sample : 04034-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	88	rVB	113323	118745	11.66%	1.487%
2	1.532	148	153	163	rVB	104454	118820	11.66%	1.488%
3	2.063	310	318	330	rVB	198341	281938	27.68%	3.531%
4	2.809	547	550	556	rBV6	1094	1361	0.13%	0.017%
5	3.011	610	613	615	rBV3	850	483	0.05%	0.006%
6	3.043	621	623	625	rBV3	894	350	0.03%	0.004%
7	3.159	657	659	664	rBV5	785	705	0.07%	0.009%
8	3.243	683	685	687	rBV3	814	484	0.05%	0.006%
9	3.285	695	698	700	rBV3	832	494	0.05%	0.006%
10	3.542	776	778	783	rBV4	560	337	0.03%	0.004%
11	3.613	796	800	801	rBV4	280	196	0.02%	0.002%
12	3.651	808	812	816	rBV4	889	662	0.06%	0.008%
13	3.677	816	820	823	rBV4	684	593	0.06%	0.007%
14	3.748	838	842	843	rBV4	715	416	0.04%	0.005%
15	3.796	848	857	886	rBV	71681	196903	19.33%	2.466%
16	4.162	969	971	973	rBV3	762	437	0.04%	0.005%
17	4.252	986	999	1024	rBV	150622	390255	38.31%	4.888%
18	4.809	1168	1172	1177	rVB7	1076	1171	0.11%	0.015%
19	4.838	1179	1181	1183	rBV3	486	324	0.03%	0.004%
20	4.960	1203	1219	1246	rBV2	384395	1018707	100.00%	12.759%
21	5.400	1352	1356	1360	rBV7	1445	1248	0.12%	0.016%
22	5.538	1387	1399	1420	rBV	317910	654333	64.23%	8.195%
23	5.828	1479	1489	1511	rBV2	40765	86251	8.47%	1.080%
24	5.992	1528	1540	1573	rBV	228832	480951	47.21%	6.024%
25	6.416	1668	1672	1678	rVB6	987	1122	0.11%	0.014%
26	6.445	1678	1681	1682	rBV3	685	376	0.04%	0.005%
27	6.664	1745	1749	1755	rVB8	810	813	0.08%	0.010%
28	6.686	1755	1756	1759	rVB3	493	163	0.02%	0.002%
29	6.706	1759	1762	1764	rBV4	903	499	0.05%	0.006%
30	6.815	1794	1796	1799	rBV3	740	520	0.05%	0.007%
31	6.854	1806	1808	1810	rBV2	739	391	0.04%	0.005%
32	6.918	1817	1828	1854	rBV	134971	261819	25.70%	3.279%
33	7.246	1919	1930	1958	rBV	466186	832216	81.69%	10.423%
34	7.448	1990	1993	1997	rBV7	1408	1173	0.12%	0.015%
35	7.558	2018	2027	2052	rBV	93709	171727	16.86%	2.151%
36	7.882	2119	2128	2135	rBV3	3342	5831	0.57%	0.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031868.D
 Acq On : 23 Aug 2023 14:27
 Operator : SY/MD
 Sample : 04034-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.911	2135	2137	2144	rVB7	1527	1191	0.12%	0.015%
38	7.944	2144	2147	2148	rBV3	795	366	0.04%	0.005%
39	8.030	2165	2174	2208	rBV	167283	355534	34.90%	4.453%
40	8.416	2292	2294	2296	rBV3	335	178	0.02%	0.002%
41	8.474	2308	2312	2317	rVB8	872	892	0.09%	0.011%
42	8.561	2337	2339	2341	rBV2	496	229	0.02%	0.003%
43	8.622	2354	2358	2359	rBV3	699	471	0.05%	0.006%
44	8.644	2363	2365	2369	rBV4	649	501	0.05%	0.006%
45	8.680	2374	2376	2379	rBV4	637	473	0.05%	0.006%
46	8.789	2398	2410	2437	rBV	490012	831827	81.66%	10.418%
47	9.014	2478	2480	2481	rBV2	590	219	0.02%	0.003%
48	9.085	2500	2502	2503	rBV3	860	363	0.04%	0.005%
49	9.197	2535	2537	2539	rBV3	619	275	0.03%	0.003%
50	9.252	2552	2554	2555	rBV2	560	251	0.02%	0.003%
51	9.294	2565	2567	2568	rBV2	492	197	0.02%	0.002%
52	9.406	2598	2602	2604	rBV4	897	771	0.08%	0.010%
53	9.445	2607	2614	2619	rVB8	1342	1267	0.12%	0.016%
54	9.480	2619	2625	2626	rBV6	833	746	0.07%	0.009%
55	9.718	2697	2699	2702	rBV3	664	461	0.05%	0.006%
56	9.767	2708	2714	2718	rBV8	1632	1823	0.18%	0.023%
57	9.876	2742	2748	2751	rBV7	1410	1609	0.16%	0.020%
58	9.934	2761	2766	2769	rBV6	947	1003	0.10%	0.013%
59	9.995	2783	2785	2787	rBV3	505	289	0.03%	0.004%
60	10.075	2807	2810	2812	rBV3	967	563	0.06%	0.007%
61	10.156	2824	2835	2854	rBV	253766	407554	40.01%	5.104%
62	10.329	2882	2889	2901	rVB2	8402	12988	1.27%	0.163%
63	10.378	2901	2904	2905	rBV3	716	400	0.04%	0.005%
64	10.413	2912	2915	2916	rBV3	478	225	0.02%	0.003%
65	10.455	2927	2928	2930	rVB2	655	204	0.02%	0.003%
66	10.548	2955	2957	2958	rBV2	502	184	0.02%	0.002%
67	10.593	2966	2971	2973	rBV4	854	632	0.06%	0.008%
68	10.615	2973	2978	2981	rVB4	802	786	0.08%	0.010%
69	10.638	2983	2985	2987	rVV3	836	318	0.03%	0.004%
70	10.654	2987	2990	2992	rVB3	732	397	0.04%	0.005%
71	10.667	2992	2994	2997	rBV4	1146	614	0.06%	0.008%
72	10.683	2997	2999	3002	rBV3	442	241	0.02%	0.003%
73	10.747	3016	3019	3025	rVB5	765	575	0.06%	0.007%
74	10.779	3025	3029	3035	rVB7	871	856	0.08%	0.011%
75	10.812	3035	3039	3042	rBV5	813	720	0.07%	0.009%
76	10.834	3042	3046	3047	rBV3	587	468	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031868.D
 Acq On : 23 Aug 2023 14:27
 Operator : SY/MD
 Sample : 04034-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.911	3065	3070	3073	rBV7	1339	1255	0.12%	0.016%
78	10.979	3088	3091	3092	rBV	677	372	0.04%	0.005%
79	11.059	3112	3116	3118	rBV3	738	500	0.05%	0.006%
80	11.098	3125	3128	3130	rBV4	1071	864	0.08%	0.011%
81	11.188	3145	3156	3182	rBV	572821	896050	87.96%	11.223%
82	11.410	3222	3225	3230	rBV5	944	976	0.10%	0.012%
83	11.448	3235	3237	3241	rVB4	431	286	0.03%	0.004%
84	11.477	3244	3246	3249	rBV4	442	381	0.04%	0.005%
85	11.513	3249	3257	3261	rBV8	3011	5210	0.51%	0.065%
86	11.564	3262	3273	3293	rVB	502448	800580	78.59%	10.027%
87	12.082	3431	3434	3436	rBV3	908	541	0.05%	0.007%
88	12.300	3495	3502	3512	rBV7	4649	8220	0.81%	0.103%
89	12.397	3530	3532	3536	rVV4	721	515	0.05%	0.006%
90	12.429	3540	3542	3545	rVB3	669	366	0.04%	0.005%
91	12.590	3587	3592	3596	rBV7	2182	1846	0.18%	0.023%
92	12.644	3607	3609	3611	rBV3	893	376	0.04%	0.005%
93	12.834	3664	3668	3669	rBV3	819	628	0.06%	0.008%
94	13.059	3734	3738	3743	rBV7	995	1068	0.10%	0.013%
95	13.548	3887	3890	3891	rBV3	564	367	0.04%	0.005%
96	13.580	3896	3900	3901	rBV5	1241	704	0.07%	0.009%
97	13.943	4011	4013	4016	rBV3	615	308	0.03%	0.004%
98	14.217	4096	4098	4100	rBV3	941	495	0.05%	0.006%
99	14.467	4174	4176	4181	rBV5	851	490	0.05%	0.006%
100	14.914	4313	4315	4317	rBV3	882	529	0.05%	0.007%




Sum of corrected areas: 7984402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031868.D
Acq On : 23 Aug 2023 14:27
Operator : SY/MD
Sample : 04034-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

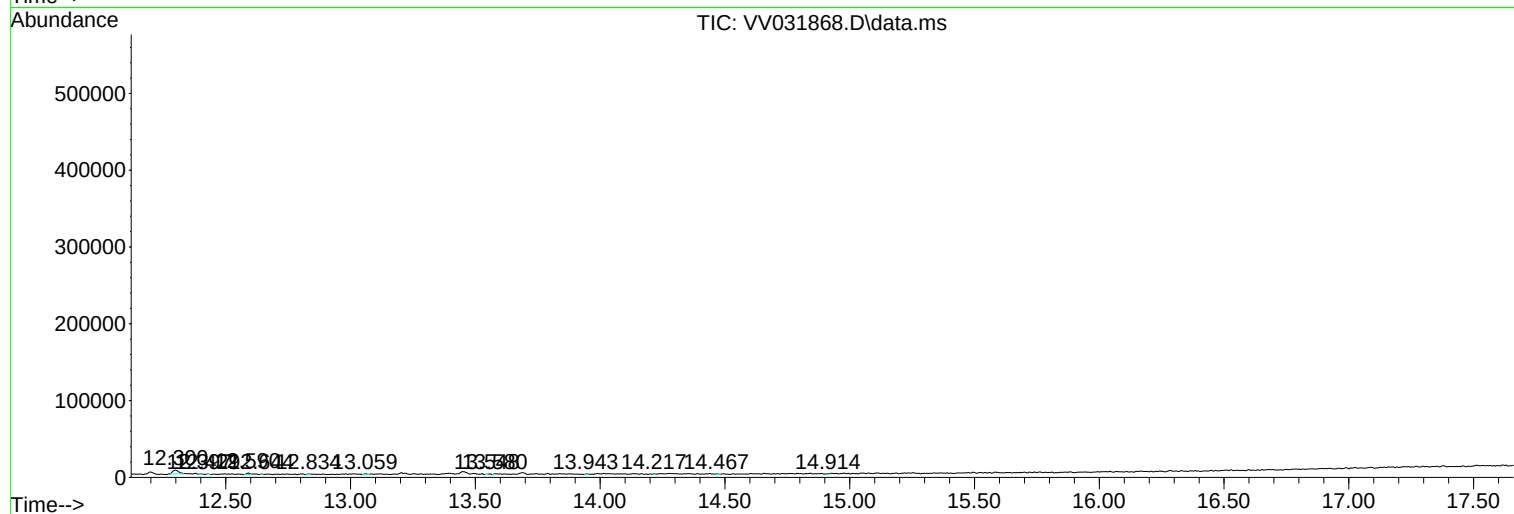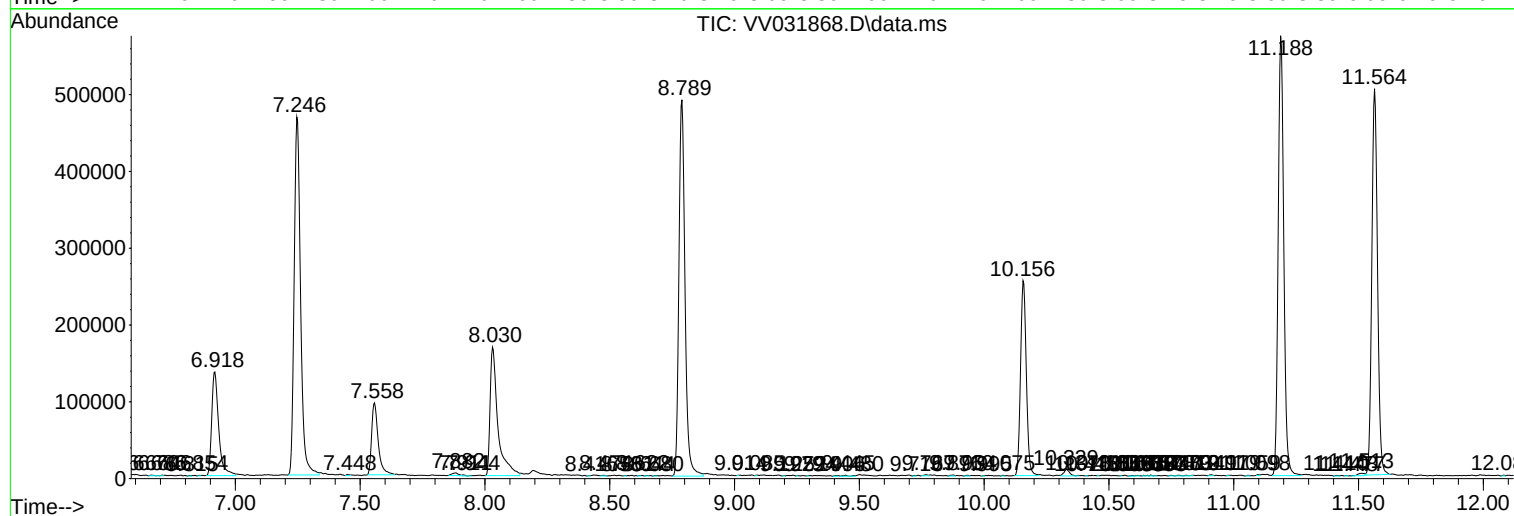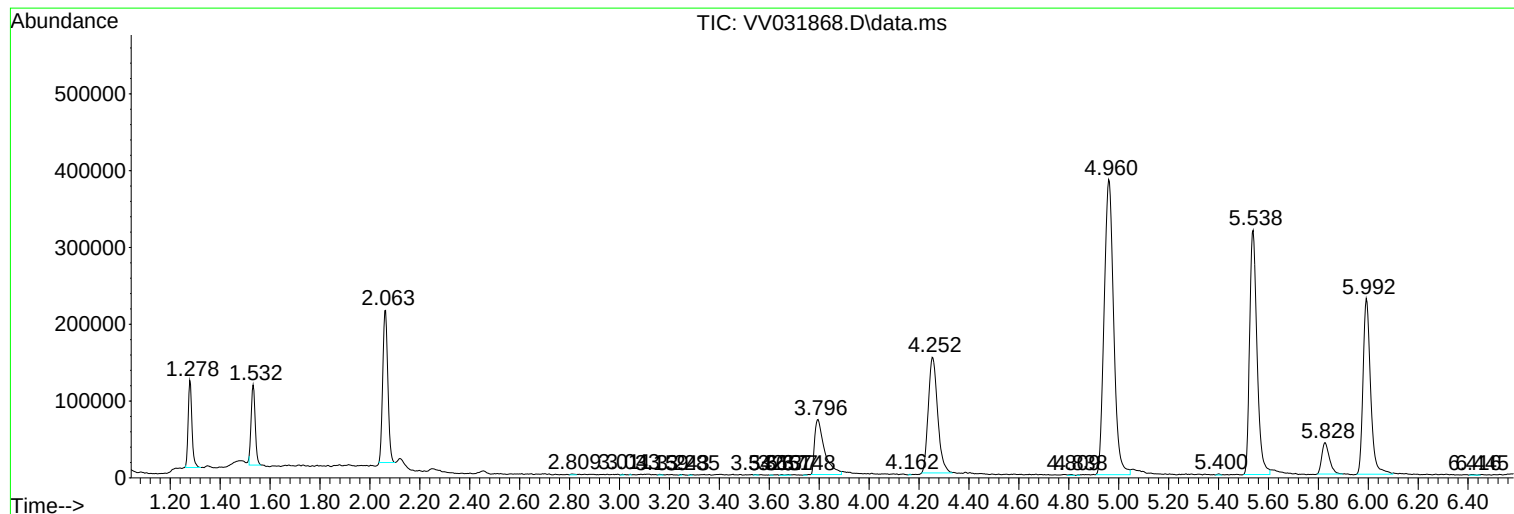

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031868.D
Acq On : 23 Aug 2023 14:27
Operator : SY/MD
Sample : 04034-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031868.D
Acq On : 23 Aug 2023 14:27
Operator : SY/MD
Sample : 04034-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc