

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031869.D
 Acq On : 23 Aug 2023 14:50
 Operator : SY/MD
 Sample : 04108-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	89	rVB	118397	122559	11.50%	1.469%
2	1.532	147	153	167	rVB	112763	134407	12.61%	1.611%
3	2.060	310	317	330	rVB	210569	302769	28.40%	3.628%
4	2.838	557	559	563	rBV4	771	591	0.06%	0.007%
5	3.208	668	674	678	rBV6	1252	1218	0.11%	0.015%
6	3.233	678	682	685	rBV5	796	741	0.07%	0.009%
7	3.487	757	761	766	rBV6	967	1056	0.10%	0.013%
8	3.619	799	802	807	rBV5	793	621	0.06%	0.007%
9	3.693	823	825	826	rVB2	511	118	0.01%	0.001%
10	3.703	826	828	831	rBV3	507	387	0.04%	0.005%
11	3.793	847	856	884	rBV	74342	206653	19.38%	2.476%
12	4.253	984	999	1023	rBV	161928	425760	39.94%	5.102%
13	4.568	1094	1097	1100	rBV3	651	533	0.05%	0.006%
14	4.638	1116	1119	1121	rBV3	758	477	0.04%	0.006%
15	4.870	1189	1191	1194	rBV4	732	504	0.05%	0.006%
16	4.902	1197	1201	1202	rBV3	813	625	0.06%	0.007%
17	4.960	1203	1219	1244	rBV2	404491	1066122	100.00%	12.775%
18	5.259	1309	1312	1314	rBV3	1152	665	0.06%	0.008%
19	5.539	1387	1399	1421	rBV	334038	686054	64.35%	8.221%
20	5.825	1478	1488	1506	rBV	39934	85284	8.00%	1.022%
21	5.992	1526	1540	1561	rBV	238205	500011	46.90%	5.991%
22	6.269	1624	1626	1627	rBV2	561	181	0.02%	0.002%
23	6.301	1633	1636	1641	rBV6	797	702	0.07%	0.008%
24	6.362	1649	1655	1658	rBV6	821	948	0.09%	0.011%
25	6.420	1670	1673	1675	rBV3	805	450	0.04%	0.005%
26	6.510	1699	1701	1704	rBV3	580	213	0.02%	0.003%
27	6.535	1704	1709	1710	rBV5	629	516	0.05%	0.006%
28	6.735	1768	1771	1774	rBV3	611	455	0.04%	0.005%
29	6.777	1779	1784	1787	rBV3	703	618	0.06%	0.007%
30	6.918	1817	1828	1859	rBV	141820	277474	26.03%	3.325%
31	7.246	1919	1930	1960	rBV	491079	873954	81.98%	10.472%
32	7.555	2017	2026	2052	rBV	101426	184116	17.27%	2.206%
33	7.998	2160	2164	2165	rBV4	803	493	0.05%	0.006%
34	8.031	2166	2174	2205	rVV	175204	360846	33.85%	4.324%
35	8.532	2328	2330	2331	rBV2	881	394	0.04%	0.005%
36	8.593	2346	2349	2351	rBV2	672	379	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031869.D
 Acq On : 23 Aug 2023 14:50
 Operator : SY/MD
 Sample : 04108-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	8.651	2364	2367	2370	rBV4	780	491	0.05%	0.006%
38	8.725	2388	2390	2393	rBV4	716	469	0.04%	0.006%
39	8.786	2399	2409	2438	rBV	511591	857298	80.41%	10.272%
40	9.043	2487	2489	2490	rBV	781	396	0.04%	0.005%
41	9.198	2536	2537	2538	rBV	497	188	0.02%	0.002%
42	9.259	2553	2556	2557	rBV2	404	209	0.02%	0.003%
43	9.275	2558	2561	2566	rVV5	1333	1323	0.12%	0.016%
44	9.313	2570	2573	2575	rBV4	581	411	0.04%	0.005%
45	9.333	2576	2579	2580	rBV2	553	281	0.03%	0.003%
46	9.410	2600	2603	2607	rBV4	816	736	0.07%	0.009%
47	9.432	2607	2610	2612	rBV4	746	505	0.05%	0.006%
48	9.590	2657	2659	2660	rBV2	853	349	0.03%	0.004%
49	9.603	2662	2663	2669	rVB6	1131	903	0.08%	0.011%
50	9.632	2669	2672	2675	rBV3	560	426	0.04%	0.005%
51	9.680	2685	2687	2689	rBV4	511	226	0.02%	0.003%
52	9.738	2702	2705	2709	rVB6	681	423	0.04%	0.005%
53	9.767	2709	2714	2718	rBV5	682	799	0.07%	0.010%
54	9.857	2740	2742	2745	rBV3	610	369	0.03%	0.004%
55	9.940	2763	2768	2771	rBV6	968	905	0.08%	0.011%
56	9.966	2774	2776	2777	rBV2	552	207	0.02%	0.002%
57	10.037	2792	2798	2802	rBV6	1082	1024	0.10%	0.012%
58	10.079	2809	2811	2814	rBV4	776	384	0.04%	0.005%
59	10.098	2814	2817	2819	rBV2	767	537	0.05%	0.006%
60	10.156	2825	2835	2856	rVB	272767	437506	41.04%	5.242%
61	10.301	2876	2880	2882	rBV4	762	511	0.05%	0.006%
62	10.333	2882	2890	2898	rVB5	3022	5363	0.50%	0.064%
63	10.400	2909	2911	2914	rBV5	534	317	0.03%	0.004%
64	10.445	2922	2925	2928	rVB4	873	579	0.05%	0.007%
65	10.461	2928	2930	2931	rBV	788	326	0.03%	0.004%
66	10.571	2960	2964	2967	rVB5	505	344	0.03%	0.004%
67	10.590	2967	2970	2972	rBV4	497	340	0.03%	0.004%
68	10.661	2990	2992	2993	rBV2	489	190	0.02%	0.002%
69	10.754	3017	3021	3022	rBV4	523	321	0.03%	0.004%
70	10.792	3030	3033	3037	rVB5	1048	735	0.07%	0.009%
71	10.831	3043	3045	3050	rBV5	788	586	0.05%	0.007%
72	10.860	3050	3054	3057	rBV5	1020	925	0.09%	0.011%
73	10.915	3069	3071	3075	rBV3	1002	609	0.06%	0.007%
74	11.005	3097	3099	3101	rBV3	623	317	0.03%	0.004%
75	11.098	3126	3128	3130	rBV3	694	369	0.03%	0.004%
76	11.188	3145	3156	3179	rBV	586729	924073	86.68%	11.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031869.D
 Acq On : 23 Aug 2023 14:50
 Operator : SY/MD
 Sample : 04108-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.410	3221	3225	3229	rVB5	1026	978	0.09%	0.012%
78	11.445	3229	3236	3237	rBV5	755	815	0.08%	0.010%
79	11.506	3247	3255	3262	rBV6	4509	9007	0.84%	0.108%
80	11.564	3262	3273	3294	rVB	525681	840562	78.84%	10.072%
81	11.960	3393	3396	3398	rBV4	603	397	0.04%	0.005%
82	12.034	3417	3419	3422	rVB2	618	292	0.03%	0.003%
83	12.111	3439	3443	3445	rBV5	713	535	0.05%	0.006%
84	12.477	3556	3557	3561	rVB4	662	444	0.04%	0.005%
85	12.497	3561	3563	3565	rBV3	557	215	0.02%	0.003%
86	12.509	3565	3567	3570	rBV3	636	400	0.04%	0.005%
87	12.638	3605	3607	3608	rBV	519	221	0.02%	0.003%
88	12.776	3648	3650	3653	rBV4	991	560	0.05%	0.007%
89	12.937	3698	3700	3702	rBV2	659	350	0.03%	0.004%
90	12.969	3708	3710	3713	rBV4	442	343	0.03%	0.004%
91	13.014	3722	3724	3727	rVB2	1145	562	0.05%	0.007%
92	13.037	3727	3731	3733	rBV5	876	683	0.06%	0.008%
93	13.098	3749	3750	3751	rBV	398	98	0.01%	0.001%
94	13.210	3779	3785	3789	rBV6	1719	2104	0.20%	0.025%
95	13.452	3856	3860	3866	rVB6	2869	2837	0.27%	0.034%
96	13.561	3892	3894	3900	rVB6	937	664	0.06%	0.008%
97	13.622	3910	3913	3916	rBV4	789	620	0.06%	0.007%
98	14.172	4080	4084	4086	rBV4	843	823	0.08%	0.010%
99	14.252	4107	4109	4111	rBV3	972	539	0.05%	0.006%
100	14.397	4152	4154	4157	rBV4	649	432	0.04%	0.005%




Sum of corrected areas: 8345645

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031869.D
Acq On : 23 Aug 2023 14:50
Operator : SY/MD
Sample : 04108-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

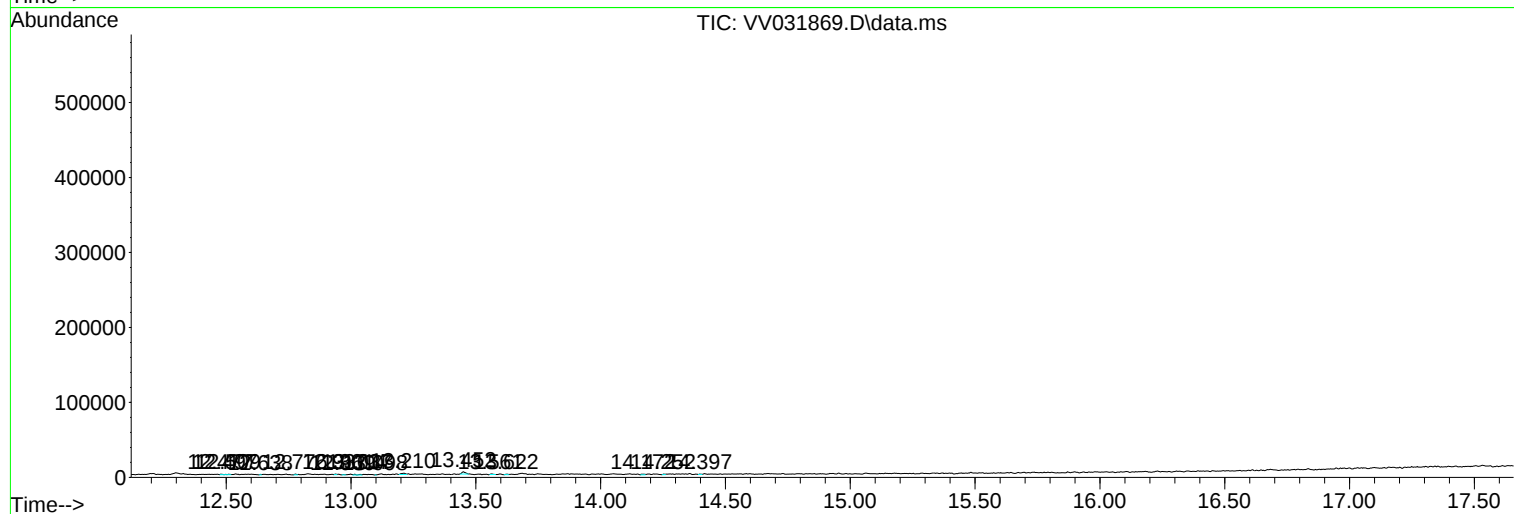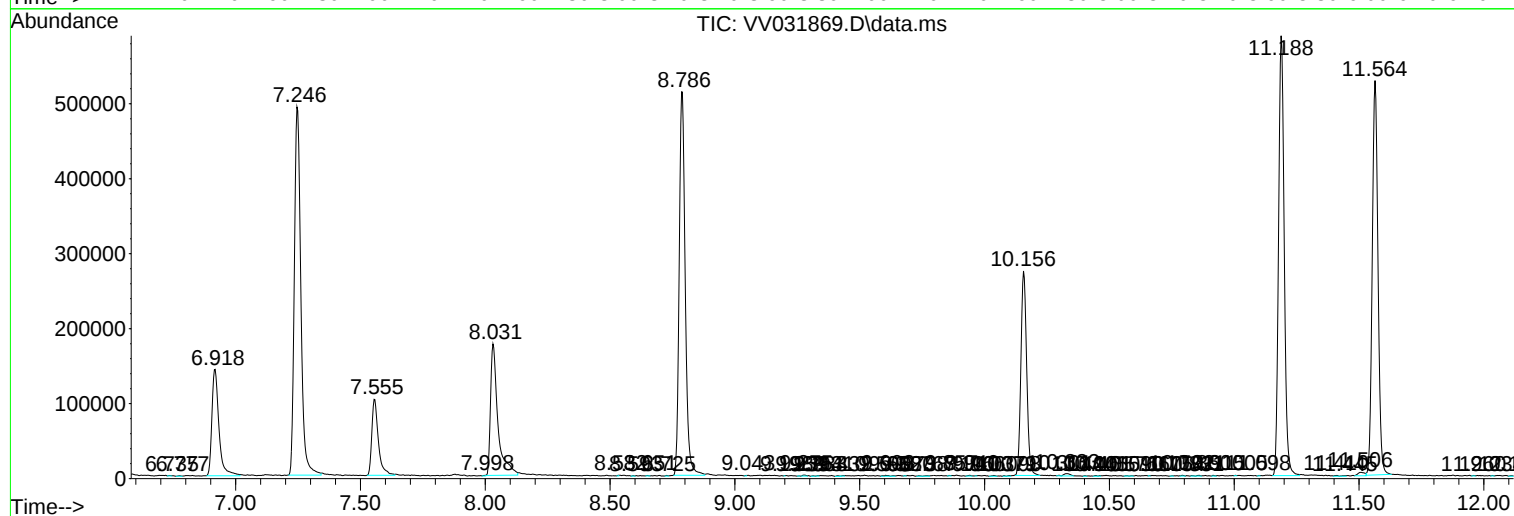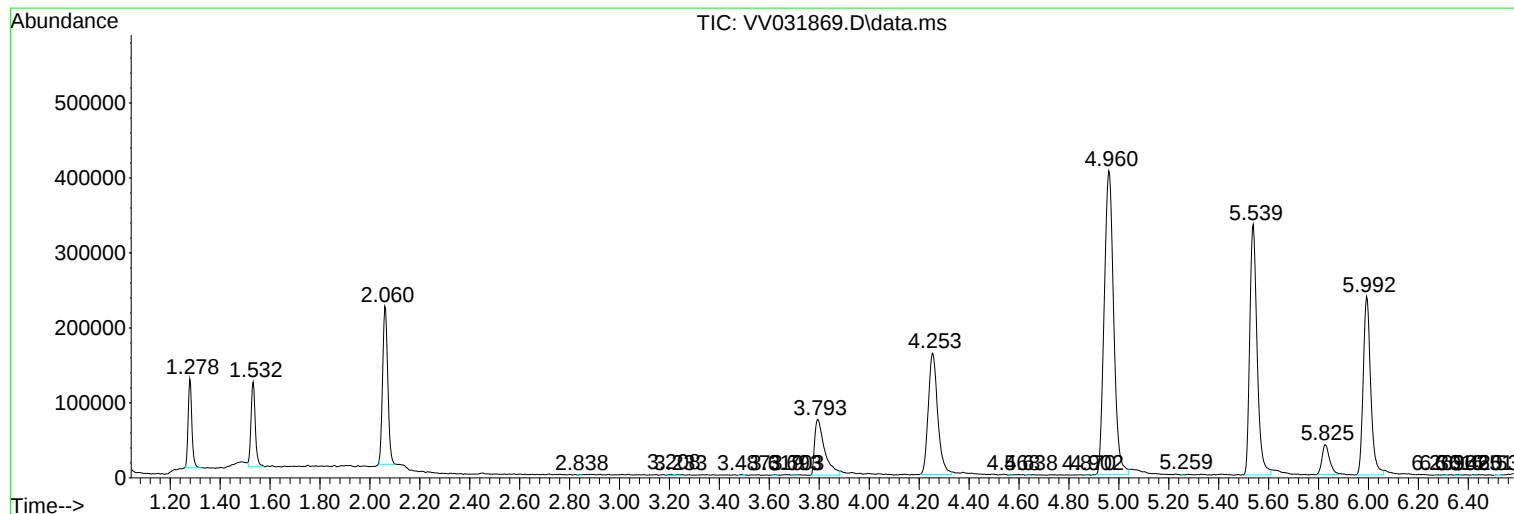

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031869.D
Acq On : 23 Aug 2023 14:50
Operator : SY/MD
Sample : 04108-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031869.D
Acq On : 23 Aug 2023 14:50
Operator : SY/MD
Sample : 04108-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc