

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031871.D
 Acq On : 23 Aug 2023 15:35
 Operator : SY/MD
 Sample : 04037-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	86	rVB	109778	117194	11.45%	1.479%
2	1.532	148	153	165	rVB	106878	121661	11.89%	1.535%
3	2.063	310	318	331	rVB	197713	280007	27.36%	3.533%
4	3.034	619	620	621	rBV	633	223	0.02%	0.003%
5	3.227	678	680	684	rBV3	634	470	0.05%	0.006%
6	3.317	706	708	709	rBV3	746	318	0.03%	0.004%
7	3.796	848	857	884	rBV	70408	192966	18.86%	2.435%
8	4.256	983	1000	1028	rBV	154490	412459	40.31%	5.204%
9	4.519	1079	1082	1084	rBV4	1106	894	0.09%	0.011%
10	4.613	1109	1111	1112	rBV3	673	277	0.03%	0.003%
11	4.658	1123	1125	1128	rBV4	725	373	0.04%	0.005%
12	4.709	1138	1141	1144	rBV3	862	685	0.07%	0.009%
13	4.741	1147	1151	1153	rVB5	763	593	0.06%	0.007%
14	4.754	1153	1155	1156	rBV3	505	189	0.02%	0.002%
15	4.851	1182	1185	1187	rBV3	533	313	0.03%	0.004%
16	4.870	1189	1191	1195	rVB4	836	542	0.05%	0.007%
17	4.960	1203	1219	1245	rBV2	386981	1023253	100.00%	12.910%
18	5.259	1310	1312	1316	rBV5	756	527	0.05%	0.007%
19	5.326	1329	1333	1337	rBV6	1013	1033	0.10%	0.013%
20	5.539	1387	1399	1425	rBV	312731	646530	63.18%	8.157%
21	5.828	1477	1489	1509	rBV2	39579	87652	8.57%	1.106%
22	5.995	1528	1541	1564	rBV	225884	472567	46.18%	5.962%
23	6.301	1633	1636	1641	rVB5	908	741	0.07%	0.009%
24	6.326	1641	1644	1646	rBV3	916	511	0.05%	0.006%
25	6.375	1656	1659	1663	rBV5	756	707	0.07%	0.009%
26	6.442	1678	1680	1683	rBV3	722	386	0.04%	0.005%
27	6.542	1708	1711	1713	rBV3	885	609	0.06%	0.008%
28	6.767	1779	1781	1785	rVB3	858	527	0.05%	0.007%
29	6.918	1818	1828	1847	rBV	134875	252618	24.69%	3.187%
30	7.246	1919	1930	1966	rBV	463908	832880	81.40%	10.508%
31	7.558	2017	2027	2048	rBV	94882	177758	17.37%	2.243%
32	7.764	2089	2091	2094	rBV3	752	467	0.05%	0.006%
33	7.863	2116	2122	2123	rBV5	1232	1264	0.12%	0.016%
34	8.034	2165	2175	2210	rBV	169575	366714	35.84%	4.627%
35	8.458	2304	2307	2311	rBV5	937	748	0.07%	0.009%
36	8.526	2327	2328	2329	rBV	567	130	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031871.D
 Acq On : 23 Aug 2023 15:35
 Operator : SY/MD
 Sample : 04037-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	8.580	2344	2345	2348	rBV3	503	164	0.02%	0.002%
38	8.625	2357	2359	2362	rBV2	466	317	0.03%	0.004%
39	8.789	2398	2410	2431	rBV	478788	799853	78.17%	10.091%
40	9.153	2520	2523	2525	rBV4	777	366	0.04%	0.005%
41	9.191	2533	2535	2539	rBV4	506	386	0.04%	0.005%
42	9.211	2539	2541	2543	rBV3	636	376	0.04%	0.005%
43	9.249	2551	2553	2555	rBV3	662	290	0.03%	0.004%
44	9.545	2643	2645	2646	rBV3	624	213	0.02%	0.003%
45	9.577	2652	2655	2661	rBV9	919	946	0.09%	0.012%
46	9.683	2685	2688	2690	rBV4	926	514	0.05%	0.006%
47	9.744	2704	2707	2708	rBV2	567	334	0.03%	0.004%
48	9.757	2708	2711	2712	rBV3	888	453	0.04%	0.006%
49	9.895	2750	2754	2755	rBV4	749	434	0.04%	0.005%
50	9.940	2764	2768	2770	rBV6	946	740	0.07%	0.009%
51	10.072	2805	2809	2812	rBV4	932	599	0.06%	0.008%
52	10.095	2812	2816	2822	rBV5	1019	1380	0.13%	0.017%
53	10.156	2823	2835	2854	rBV	262305	422944	41.33%	5.336%
54	10.333	2884	2890	2900	rVB5	3170	4800	0.47%	0.061%
55	10.465	2927	2931	2934	rBV5	849	756	0.07%	0.010%
56	10.590	2967	2970	2972	rBV4	640	404	0.04%	0.005%
57	10.622	2978	2980	2986	rVB7	725	525	0.05%	0.007%
58	10.744	3014	3018	3022	rBV7	1088	1045	0.10%	0.013%
59	10.789	3027	3032	3034	rBV5	941	747	0.07%	0.009%
60	10.857	3050	3053	3056	rBV5	1212	785	0.08%	0.010%
61	11.188	3146	3156	3178	rBV	559443	869644	84.99%	10.972%
62	11.432	3231	3232	3233	rBV	588	148	0.01%	0.002%
63	11.564	3262	3273	3293	rVB	512566	800565	78.24%	10.100%
64	11.735	3322	3326	3327	rBV2	1030	590	0.06%	0.007%
65	11.969	3397	3399	3400	rBV2	583	267	0.03%	0.003%
66	12.037	3417	3420	3425	rVB4	1004	942	0.09%	0.012%
67	12.156	3454	3457	3458	rBV3	674	434	0.04%	0.005%
68	12.198	3466	3470	3479	rVB8	1600	2593	0.25%	0.033%
69	12.236	3479	3482	3484	rBV4	1009	698	0.07%	0.009%
70	12.300	3494	3502	3512	rBV6	6158	10628	1.04%	0.134%
71	13.079	3742	3744	3745	rBV2	572	212	0.02%	0.003%
72	13.198	3779	3781	3782	rBV2	649	244	0.02%	0.003%
73	13.506	3876	3877	3878	rBV	661	228	0.02%	0.003%
74	13.616	3908	3911	3913	rBV3	723	477	0.05%	0.006%
75	13.689	3930	3934	3940	rBV9	1234	1196	0.12%	0.015%
76	13.937	4009	4011	4016	rVB6	833	577	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031871.D
Acq On : 23 Aug 2023 15:35
Operator : SY/MD
Sample : 04037-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis

77	14.194	4089	4091	4092	rBV2	758	427	0.04%	0.005%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 7926027

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031871.D
Acq On : 23 Aug 2023 15:35
Operator : SY/MD
Sample : 04037-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

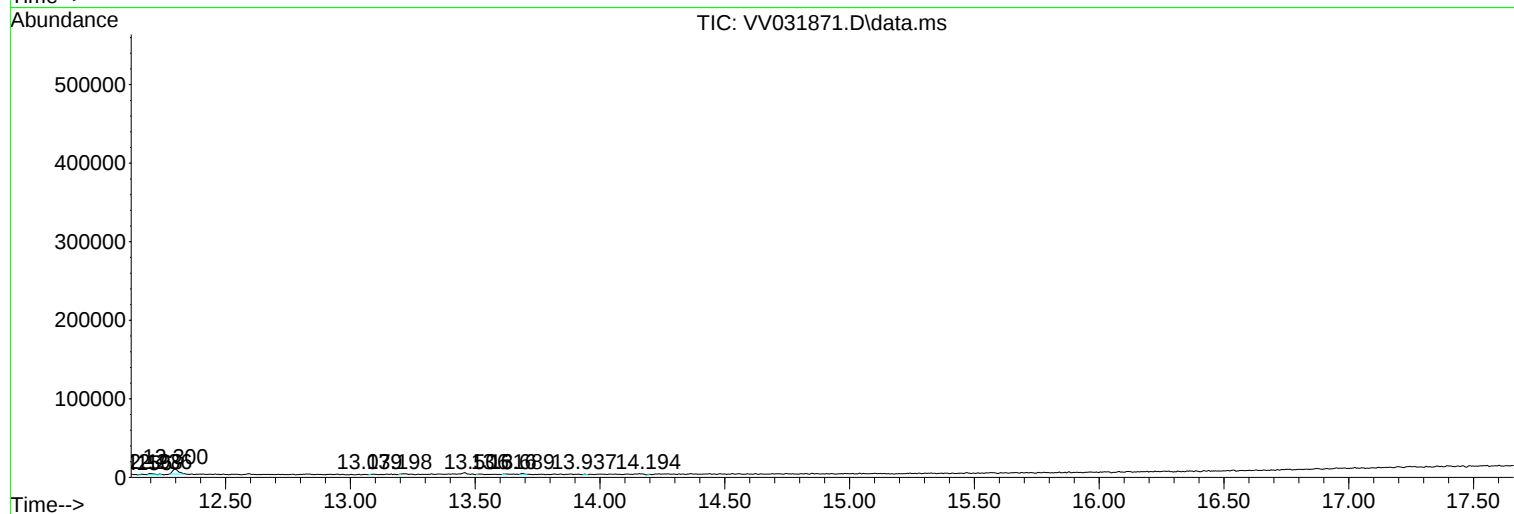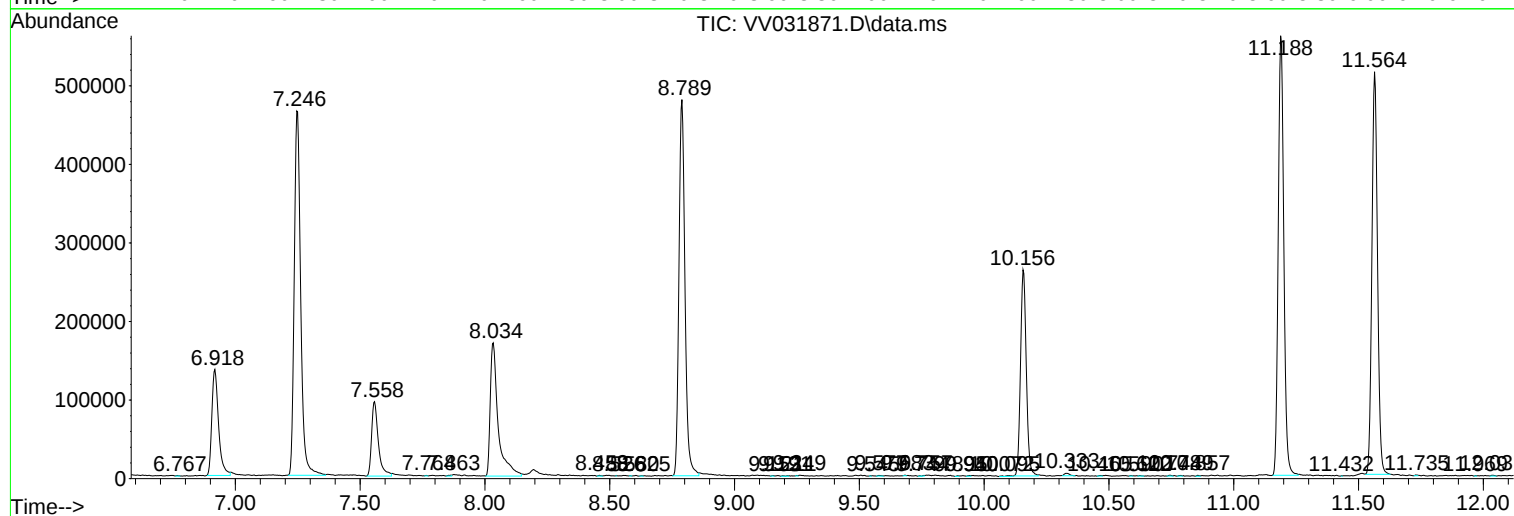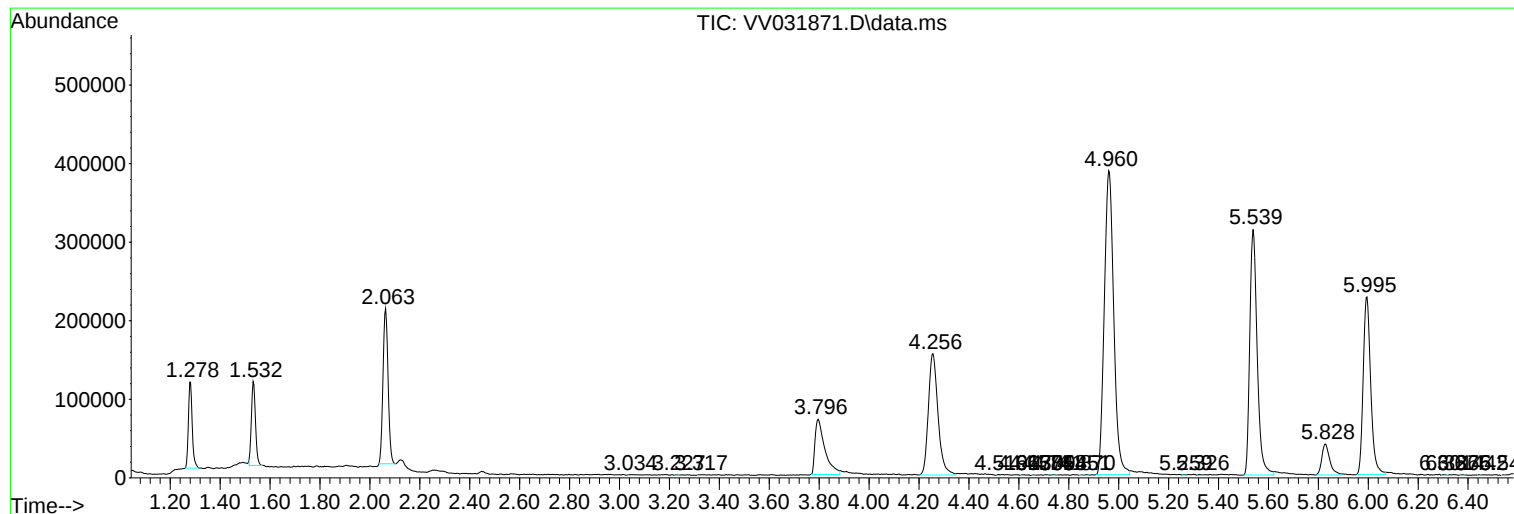

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031871.D
Acq On : 23 Aug 2023 15:35
Operator : SY/MD
Sample : 04037-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031871.D
Acq On : 23 Aug 2023 15:35
Operator : SY/MD
Sample : 04037-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc