

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031874.D
 Acq On : 23 Aug 2023 16:45
 Operator : SY/MD
 Sample : 04034-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	115959	123580	11.63%	1.525%
2	1.536	148	154	170	rVB	107357	126337	11.89%	1.560%
3	2.063	310	318	334	rVB	203323	293761	27.64%	3.626%
4	2.851	558	563	564	rBV4	1248	864	0.08%	0.011%
5	2.886	572	574	575	rBV2	760	372	0.04%	0.005%
6	2.960	590	597	600	rBV8	981	1147	0.11%	0.014%
7	3.159	657	659	661	rBV3	683	311	0.03%	0.004%
8	3.207	670	674	676	rBV4	491	315	0.03%	0.004%
9	3.262	688	691	696	rBV5	791	721	0.07%	0.009%
10	3.362	721	722	725	rBV3	498	305	0.03%	0.004%
11	3.510	766	768	771	rVB3	610	338	0.03%	0.004%
12	3.526	771	773	779	rBV4	820	909	0.09%	0.011%
13	3.587	788	792	796	rBV6	760	616	0.06%	0.008%
14	3.757	843	845	848	rVB4	846	468	0.04%	0.006%
15	3.799	848	858	891	rBV	72142	214432	20.18%	2.647%
16	4.256	985	1000	1025	rBV	157194	403036	37.93%	4.975%
17	4.680	1129	1132	1134	rVB4	762	311	0.03%	0.004%
18	4.773	1159	1161	1164	rVB3	755	329	0.03%	0.004%
19	4.799	1165	1169	1173	rVV6	1062	914	0.09%	0.011%
20	4.834	1177	1180	1183	rBV5	583	492	0.05%	0.006%
21	4.870	1188	1191	1194	rBV5	677	484	0.05%	0.006%
22	4.960	1201	1219	1254	rBV2	397469	1062639	100.00%	13.117%
23	5.539	1386	1399	1429	rBV	312117	657560	61.88%	8.117%
24	5.828	1478	1489	1509	rBV	27717	60668	5.71%	0.749%
25	5.992	1527	1540	1566	rBV	230094	491249	46.23%	6.064%
26	6.548	1711	1713	1714	rBV	909	370	0.03%	0.005%
27	6.735	1769	1771	1773	rBV3	604	314	0.03%	0.004%
28	6.825	1795	1799	1802	rBV4	557	370	0.03%	0.005%
29	6.847	1802	1806	1809	rBV5	768	703	0.07%	0.009%
30	6.918	1817	1828	1859	rBV	138462	267942	25.21%	3.307%
31	7.114	1886	1889	1890	rBV3	996	560	0.05%	0.007%
32	7.246	1918	1930	1964	rBV	474447	855014	80.46%	10.554%
33	7.481	1999	2003	2012	rBV9	1109	1527	0.14%	0.019%
34	7.558	2017	2027	2045	rBV	96957	173445	16.32%	2.141%
35	7.773	2090	2094	2100	rBV7	1108	1080	0.10%	0.013%
36	7.815	2104	2107	2109	rBV3	707	406	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031874.D
 Acq On : 23 Aug 2023 16:45
 Operator : SY/MD
 Sample : 04034-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.828	2109	2111	2113	rBV3	648	291	0.03%	0.004%
38	7.857	2118	2120	2124	rBV3	600	402	0.04%	0.005%
39	7.998	2161	2164	2165	rBV3	527	297	0.03%	0.004%
40	8.030	2165	2174	2214	rVV	174603	369743	34.79%	4.564%
41	8.574	2340	2343	2345	rBV3	572	357	0.03%	0.004%
42	8.648	2362	2366	2371	rVB6	798	880	0.08%	0.011%
43	8.719	2386	2388	2392	rVB3	638	463	0.04%	0.006%
44	8.789	2399	2410	2434	rBV	488160	806452	75.89%	9.955%
45	8.989	2470	2472	2474	rBV3	655	321	0.03%	0.004%
46	9.072	2495	2498	2502	rBV5	811	538	0.05%	0.007%
47	9.120	2511	2513	2514	rBV2	674	274	0.03%	0.003%
48	9.220	2542	2544	2548	rVB4	889	478	0.04%	0.006%
49	9.278	2559	2562	2564	rBV3	549	342	0.03%	0.004%
50	9.387	2593	2596	2599	rVB4	580	350	0.03%	0.004%
51	9.403	2599	2601	2604	rBV3	471	342	0.03%	0.004%
52	9.426	2606	2608	2610	rBV3	609	280	0.03%	0.003%
53	9.760	2709	2712	2713	rBV3	692	317	0.03%	0.004%
54	9.786	2718	2720	2723	rBV3	509	325	0.03%	0.004%
55	9.844	2736	2738	2740	rBV3	651	275	0.03%	0.003%
56	9.866	2743	2745	2748	rVV4	503	290	0.03%	0.004%
57	9.982	2777	2781	2782	rBV4	642	490	0.05%	0.006%
58	10.034	2792	2797	2802	rBV4	981	724	0.07%	0.009%
59	10.082	2806	2812	2814	rBV6	640	478	0.04%	0.006%
60	10.104	2816	2819	2821	rBV5	567	311	0.03%	0.004%
61	10.156	2821	2835	2854	rBV	291463	465734	43.83%	5.749%
62	10.474	2930	2934	2936	rBV4	716	555	0.05%	0.007%
63	10.513	2943	2946	2947	rBV3	754	431	0.04%	0.005%
64	10.619	2975	2979	2981	rBV4	775	641	0.06%	0.008%
65	10.686	2995	3000	3002	rVB6	651	516	0.05%	0.006%
66	10.722	3007	3011	3015	rVB6	782	769	0.07%	0.009%
67	10.751	3015	3020	3022	rBV4	728	753	0.07%	0.009%
68	10.799	3032	3035	3039	rBV6	603	542	0.05%	0.007%
69	10.927	3072	3075	3076	rBV2	510	328	0.03%	0.004%
70	11.075	3119	3121	3124	rBV4	436	281	0.03%	0.003%
71	11.098	3125	3128	3134	rBV7	796	671	0.06%	0.008%
72	11.130	3134	3138	3141	rBV3	1035	1011	0.10%	0.012%
73	11.188	3145	3156	3177	rBV	565243	869495	81.82%	10.733%
74	11.497	3248	3252	3253	rBV4	719	412	0.04%	0.005%
75	11.564	3261	3273	3293	rBV	518185	815129	76.71%	10.062%
76	11.757	3329	3333	3334	rBV3	690	411	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031874.D
 Acq On : 23 Aug 2023 16:45
 Operator : SY/MD
 Sample : 04034-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.876	3367	3370	3372	rBV4	714	481	0.05%	0.006%
78	11.921	3382	3384	3387	rVB	567	292	0.03%	0.004%
79	11.940	3387	3390	3391	rBV3	827	472	0.04%	0.006%
80	11.972	3397	3400	3403	rBV4	845	479	0.05%	0.006%
81	12.030	3415	3418	3421	rBV3	644	632	0.06%	0.008%
82	12.098	3433	3439	3443	rBV9	932	1012	0.10%	0.012%
83	12.136	3447	3451	3456	rBV6	1068	1364	0.13%	0.017%
84	12.185	3464	3466	3468	rBV2	664	301	0.03%	0.004%
85	12.352	3515	3518	3523	rVB6	971	887	0.08%	0.011%
86	12.423	3538	3540	3547	rBV6	614	588	0.06%	0.007%
87	12.513	3565	3568	3570	rBV3	428	318	0.03%	0.004%
88	12.522	3570	3571	3574	rVV2	673	326	0.03%	0.004%
89	12.625	3600	3603	3608	rBV6	751	493	0.05%	0.006%
90	12.712	3628	3630	3636	rVB6	733	625	0.06%	0.008%
91	12.744	3636	3640	3642	rBV6	729	537	0.05%	0.007%
92	12.776	3646	3650	3651	rBV5	809	592	0.06%	0.007%
93	12.976	3708	3712	3719	rBV8	1159	1349	0.13%	0.017%
94	13.014	3719	3724	3728	rBV5	997	1202	0.11%	0.015%
95	13.146	3762	3765	3771	rVB4	574	313	0.03%	0.004%
96	13.169	3771	3772	3775	rBV4	631	408	0.04%	0.005%
97	13.304	3810	3814	3816	rBV5	851	577	0.05%	0.007%
98	13.554	3890	3892	3895	rBV4	786	341	0.03%	0.004%
99	14.066	4049	4051	4053	rBV4	860	363	0.03%	0.004%
100	14.458	4170	4173	4176	rBV4	827	573	0.05%	0.007%




Sum of corrected areas: 8101113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031874.D
Acq On : 23 Aug 2023 16:45
Operator : SY/MD
Sample : 04034-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

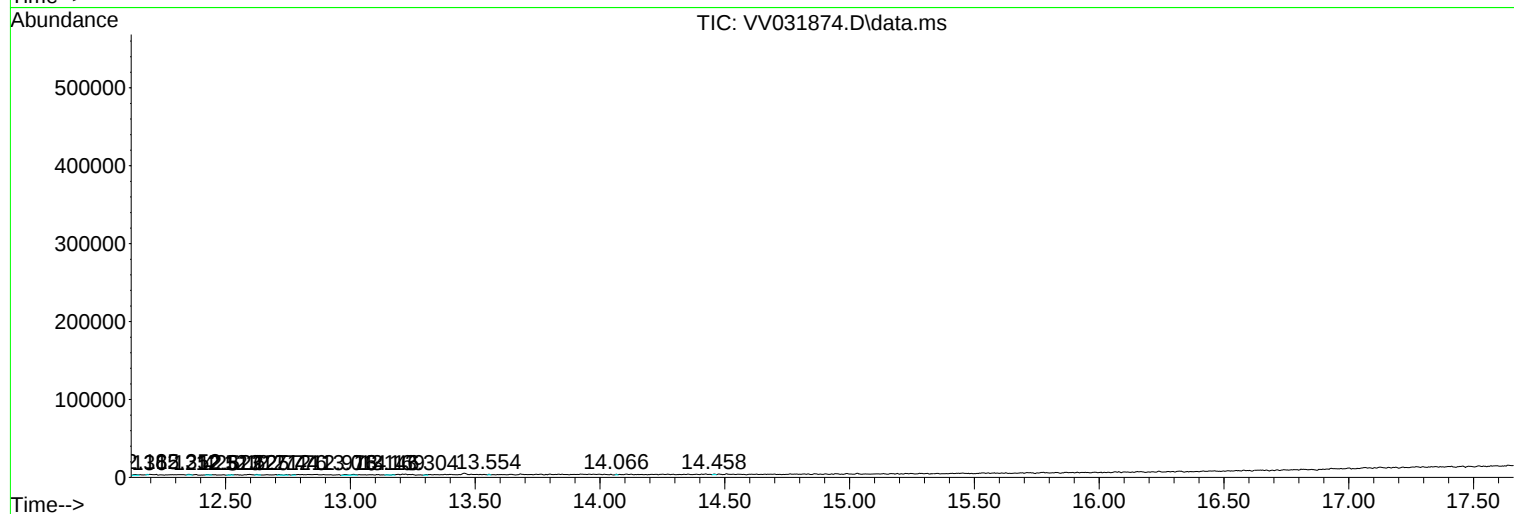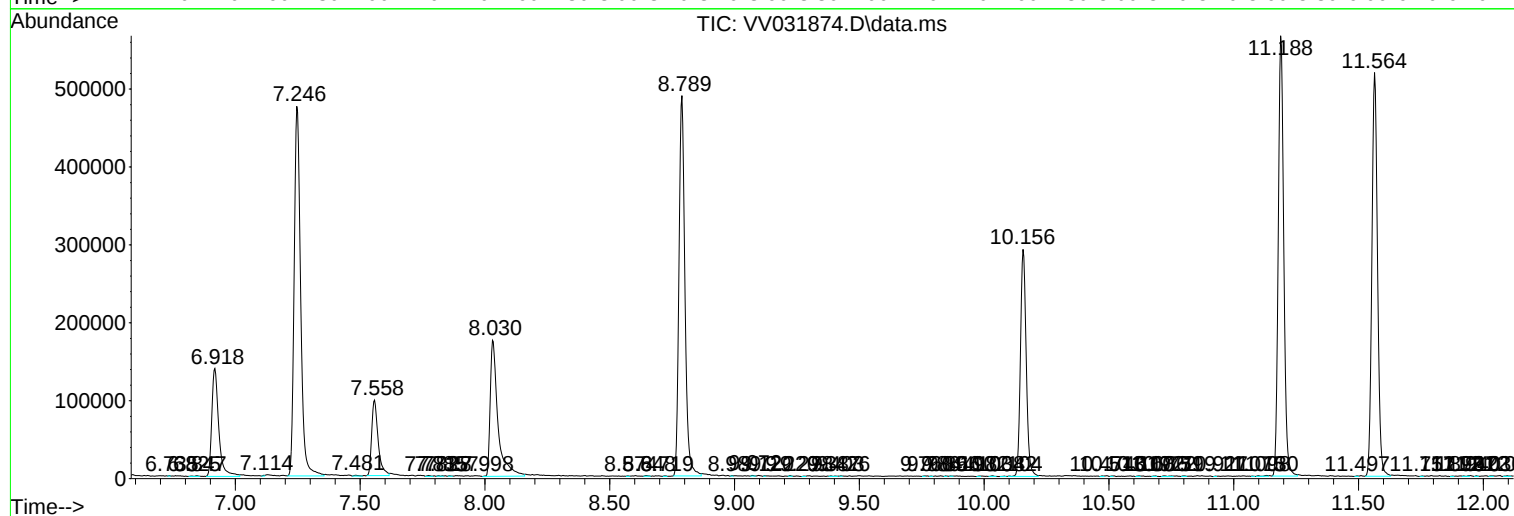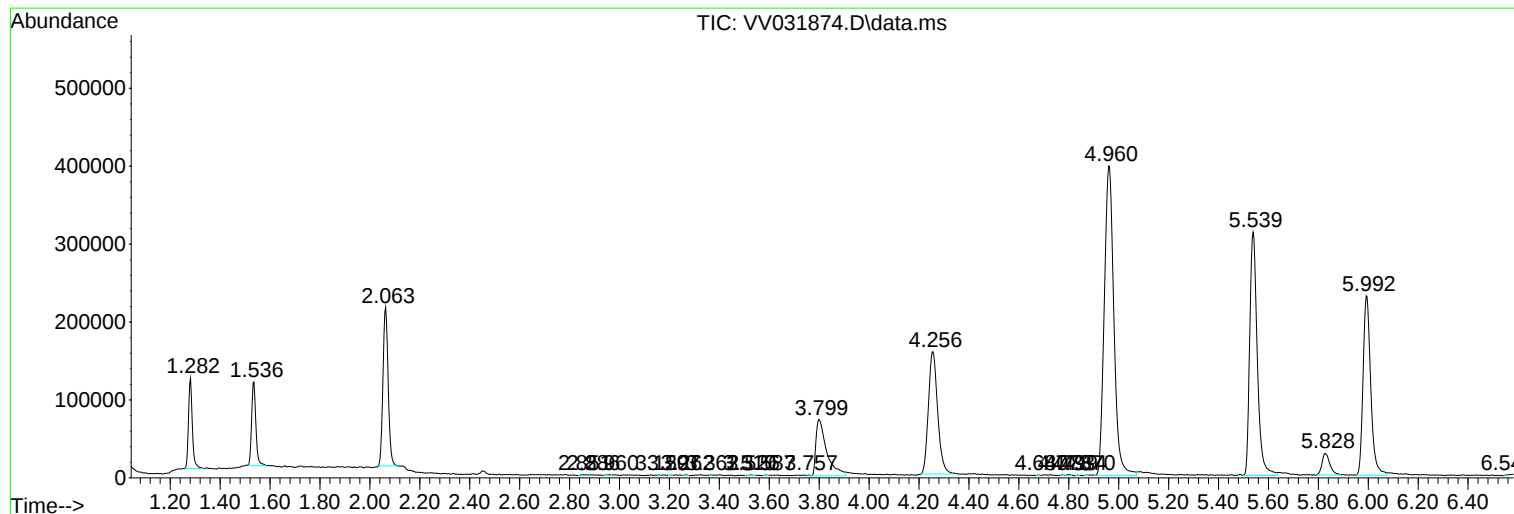

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031874.D
Acq On : 23 Aug 2023 16:45
Operator : SY/MD
Sample : 04034-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031874.D
Acq On : 23 Aug 2023 16:45
Operator : SY/MD
Sample : 04034-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc