

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031875.D
 Acq On : 23 Aug 2023 17:07
 Operator : SY/MD
 Sample : 04037-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

Signal : TIC: VV031875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	106861	110821	11.00%	1.412%
2	1.532	148	153	169	rVB	102828	122863	12.20%	1.565%
3	2.063	310	318	334	rVB	193983	280172	27.81%	3.570%
4	2.700	513	516	518	rVV4	940	546	0.05%	0.007%
5	2.847	560	562	565	rBV3	547	337	0.03%	0.004%
6	2.886	570	574	578	rBV5	966	1078	0.11%	0.014%
7	2.941	589	591	594	rBV4	744	450	0.04%	0.006%
8	3.027	613	618	621	rBV6	879	836	0.08%	0.011%
9	3.066	627	630	634	rVB4	1215	1008	0.10%	0.013%
10	3.089	634	637	639	rBV3	775	533	0.05%	0.007%
11	3.304	699	704	706	rBV5	862	741	0.07%	0.009%
12	3.359	718	721	724	rBV3	783	393	0.04%	0.005%
13	3.442	744	747	752	rVB6	777	742	0.07%	0.009%
14	3.513	765	769	770	rBV3	775	457	0.05%	0.006%
15	3.626	801	804	807	rBV5	814	525	0.05%	0.007%
16	3.712	824	831	832	rBV6	733	781	0.08%	0.010%
17	3.799	849	858	893	rVV	74022	211770	21.02%	2.698%
18	4.111	953	955	960	rBV5	987	903	0.09%	0.012%
19	4.195	979	981	985	rBV4	1256	1125	0.11%	0.014%
20	4.256	985	1000	1035	rVV	151236	397449	39.46%	5.064%
21	4.555	1090	1093	1095	rBV4	623	428	0.04%	0.005%
22	4.690	1132	1135	1138	rBV4	816	562	0.06%	0.007%
23	4.796	1166	1168	1174	rVB4	854	704	0.07%	0.009%
24	4.831	1174	1179	1182	rBV5	769	837	0.08%	0.011%
25	4.870	1185	1191	1193	rBV5	931	718	0.07%	0.009%
26	4.963	1204	1220	1250	rBV2	382190	1007288	100.00%	12.834%
27	5.539	1388	1399	1428	rBV	302208	619830	61.53%	7.897%
28	5.831	1479	1490	1512	rBV	28230	61845	6.14%	0.788%
29	5.995	1526	1541	1564	rBV	223504	473498	47.01%	6.033%
30	6.445	1679	1681	1685	rVB3	729	436	0.04%	0.006%
31	6.523	1701	1705	1710	rVB6	805	704	0.07%	0.009%
32	6.545	1710	1712	1716	rBV6	520	360	0.04%	0.005%
33	6.577	1716	1722	1725	rBV6	2032	2302	0.23%	0.029%
34	6.825	1795	1799	1802	rBV5	781	698	0.07%	0.009%
35	6.867	1808	1812	1814	rBV3	370	250	0.02%	0.003%
36	6.918	1816	1828	1851	rBV	133800	256831	25.50%	3.272%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031875.D
 Acq On : 23 Aug 2023 17:07
 Operator : SY/MD
 Sample : 04037-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.088	1878	1881	1884	rBV4	789	514	0.05%	0.007%
38	7.249	1918	1931	1958	rBV	464527	825474	81.95%	10.517%
39	7.558	2017	2027	2047	rBV2	95694	172883	17.16%	2.203%
40	7.863	2118	2122	2123	rBV3	984	628	0.06%	0.008%
41	7.947	2145	2148	2150	rBV3	732	352	0.03%	0.004%
42	8.030	2165	2174	2210	rBV	174384	364693	36.21%	4.647%
43	8.384	2281	2284	2289	rBV5	1050	734	0.07%	0.009%
44	8.629	2358	2360	2363	rBV4	715	394	0.04%	0.005%
45	8.719	2384	2388	2391	rBV3	943	890	0.09%	0.011%
46	8.789	2398	2410	2438	rBV	473607	786557	78.09%	10.021%
47	9.185	2530	2533	2535	rBV4	842	652	0.06%	0.008%
48	9.239	2548	2550	2551	rBV2	482	260	0.03%	0.003%
49	9.294	2565	2567	2568	rBV2	829	416	0.04%	0.005%
50	9.336	2578	2580	2584	rBV5	445	305	0.03%	0.004%
51	9.407	2600	2602	2605	rVB4	697	451	0.04%	0.006%
52	9.426	2605	2608	2610	rBV3	527	316	0.03%	0.004%
53	9.490	2624	2628	2632	rBV7	628	658	0.07%	0.008%
54	9.522	2637	2638	2642	rVB3	567	274	0.03%	0.003%
55	9.545	2642	2645	2648	rBV4	619	406	0.04%	0.005%
56	9.667	2678	2683	2684	rBV3	706	538	0.05%	0.007%
57	9.693	2688	2691	2695	rBV4	635	629	0.06%	0.008%
58	9.728	2700	2702	2708	rBV4	828	530	0.05%	0.007%
59	9.818	2727	2730	2732	rBV4	630	448	0.04%	0.006%
60	9.866	2742	2745	2748	rBV5	883	766	0.08%	0.010%
61	10.024	2788	2794	2798	rBV7	1045	1024	0.10%	0.013%
62	10.075	2805	2810	2811	rBV2	527	478	0.05%	0.006%
63	10.156	2824	2835	2855	rBV	282023	454446	45.12%	5.790%
64	10.448	2923	2926	2930	rBV5	743	567	0.06%	0.007%
65	10.474	2930	2934	2935	rBV3	800	438	0.04%	0.006%
66	10.516	2943	2947	2948	rBV5	451	351	0.03%	0.004%
67	10.635	2980	2984	2986	rBV4	620	435	0.04%	0.006%
68	10.670	2993	2995	2999	rVB4	491	317	0.03%	0.004%
69	10.696	2999	3003	3005	rBV5	317	263	0.03%	0.003%
70	10.770	3023	3026	3029	rVB4	897	513	0.05%	0.007%
71	10.960	3080	3085	3087	rBV5	693	625	0.06%	0.008%
72	11.001	3095	3098	3100	rBV3	804	589	0.06%	0.008%
73	11.079	3119	3122	3125	rBV4	439	383	0.04%	0.005%
74	11.188	3144	3156	3178	rBV	551440	855269	84.91%	10.897%
75	11.403	3220	3223	3226	rBV2	872	722	0.07%	0.009%
76	11.445	3234	3236	3239	rBV4	679	331	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
 Data File : VV031875.D
 Acq On : 23 Aug 2023 17:07
 Operator : SY/MD
 Sample : 04037-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.506	3253	3255	3258	rBV4	969	546	0.05%	0.007%
78	11.564	3261	3273	3294	rBV	502331	800697	79.49%	10.202%
79	11.931	3383	3387	3388	rBV4	501	401	0.04%	0.005%
80	12.062	3426	3428	3433	rBV3	424	288	0.03%	0.004%
81	12.130	3444	3449	3450	rBV4	788	503	0.05%	0.006%
82	12.159	3456	3458	3461	rBV4	465	256	0.03%	0.003%
83	12.284	3494	3497	3500	rBV4	619	412	0.04%	0.005%
84	12.326	3507	3510	3513	rVV5	731	418	0.04%	0.005%
85	12.513	3566	3568	3570	rVV2	562	266	0.03%	0.003%
86	12.590	3589	3592	3594	rBV4	731	491	0.05%	0.006%
87	12.834	3666	3668	3671	rBV2	864	560	0.06%	0.007%
88	12.898	3685	3688	3694	rVB4	895	817	0.08%	0.010%
89	12.953	3703	3705	3709	rBV3	569	353	0.04%	0.004%
90	12.992	3714	3717	3724	rBV7	773	985	0.10%	0.013%
91	13.043	3730	3733	3734	rBV4	481	299	0.03%	0.004%
92	13.140	3759	3763	3766	rBV4	760	688	0.07%	0.009%
93	13.162	3769	3770	3773	rBV3	587	354	0.04%	0.005%
94	13.349	3821	3828	3829	rBV6	488	507	0.05%	0.006%
95	13.445	3856	3858	3859	rBV2	1021	461	0.05%	0.006%
96	13.513	3877	3879	3883	rBV4	495	276	0.03%	0.004%
97	13.538	3883	3887	3889	rVV3	640	406	0.04%	0.005%
98	13.587	3899	3902	3903	rBV2	838	494	0.05%	0.006%
99	13.879	3991	3993	3995	rBV2	595	248	0.02%	0.003%
100	13.934	4007	4010	4013	rBV4	874	672	0.07%	0.009%




Sum of corrected areas: 7848738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031875.D
Acq On : 23 Aug 2023 17:07
Operator : SY/MD
Sample : 04037-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

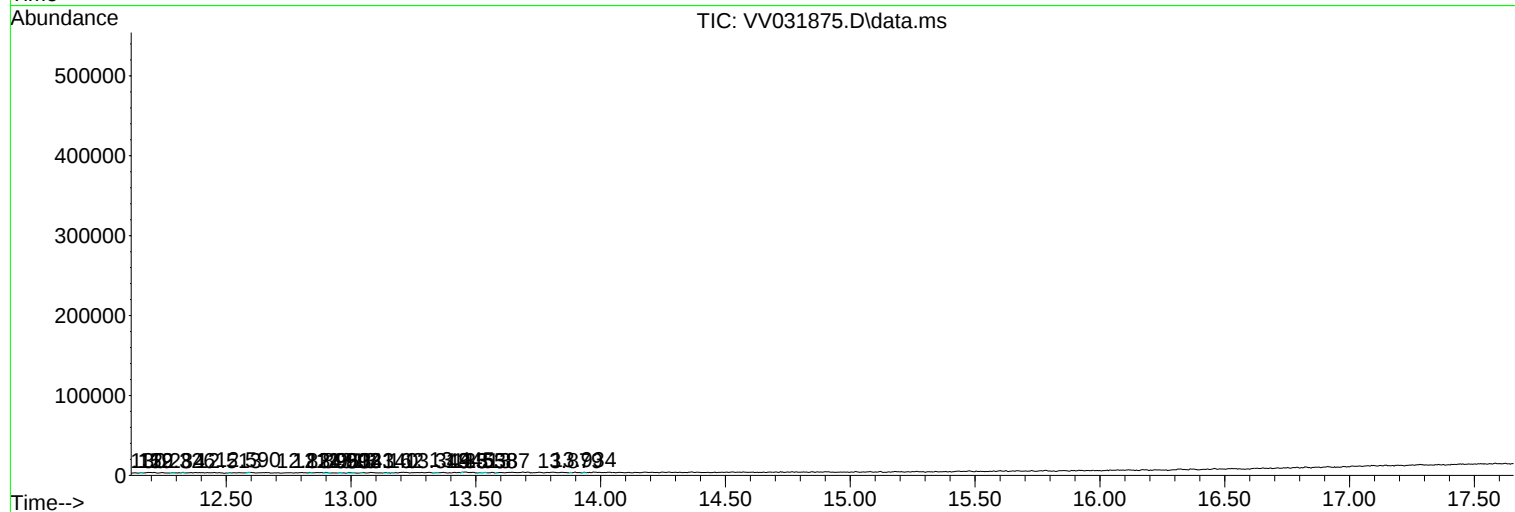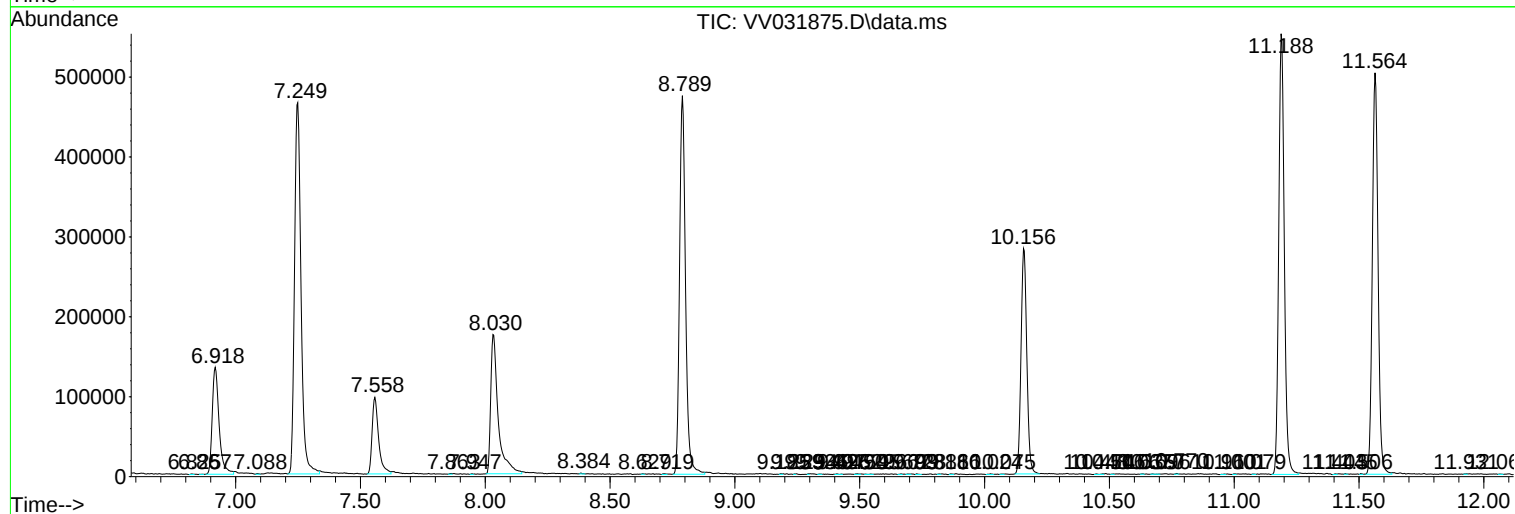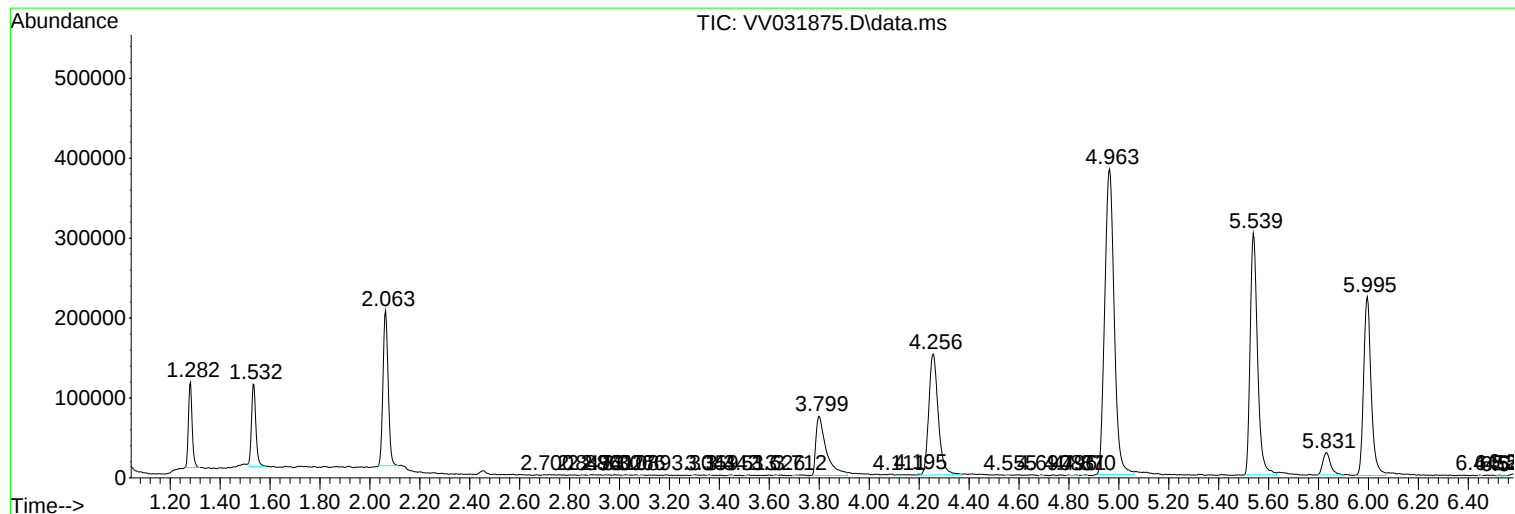

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031875.D
Acq On : 23 Aug 2023 17:07
Operator : SY/MD
Sample : 04037-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031875.D
Acq On : 23 Aug 2023 17:07
Operator : SY/MD
Sample : 04037-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc