


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082323\
Data File : VV031855.D
Acq On : 23 Aug 2023 09:09
Operator : SY/MD
Sample : BFB205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Thu Aug 24 01:40:47 2023

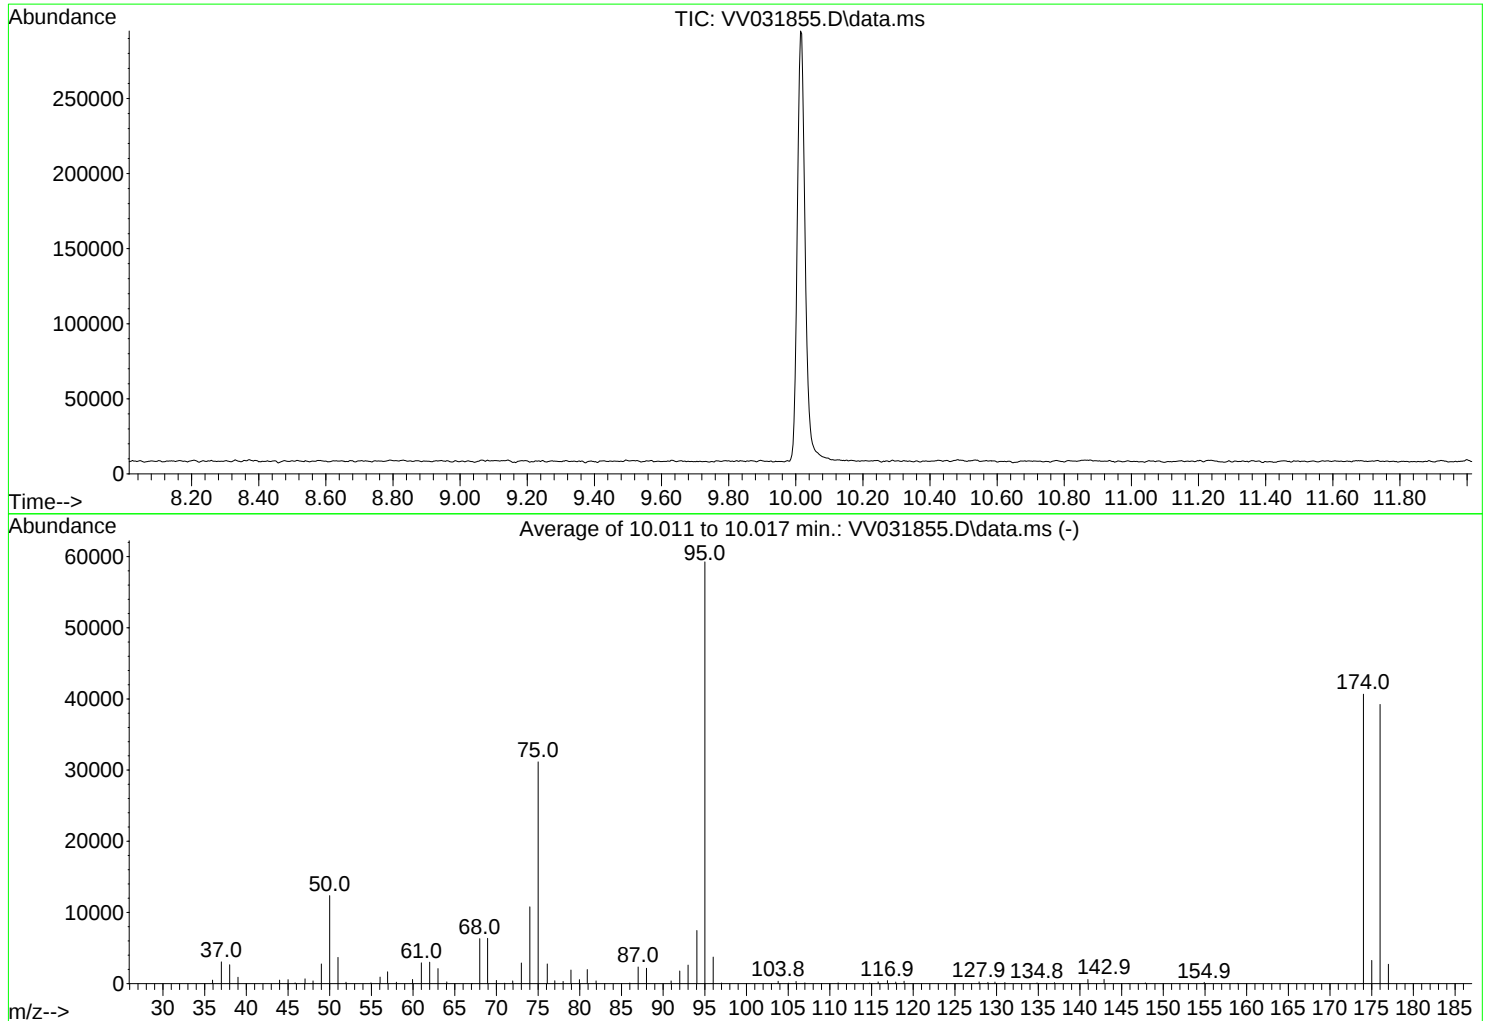

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	12365	PASS
75	95	30	80	52.6	31147	PASS
95	95	100	100	100.0	59259	PASS
96	95	5	9	6.3	3722	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.6	40675	PASS
175	174	5	9	8.0	3264	PASS
176	174	95	105	96.4	39224	PASS
177	176	5	10	6.9	2726	PASS

m/z	Abundance
35.80	104.0
38.10	121.0
39.00	323.0
40.00	289.0
41.00	619.0
42.00	261.0
43.00	537.0
44.00	2394.0
45.00	242.0
50.00	107.0
53.00	115.0
54.00	140.0
54.90	399.0
56.10	193.0
56.90	310.0
59.90	171.0
67.00	202.0
68.00	141.0
68.90	252.0
70.00	138.0
71.00	175.0
73.10	109.0
77.10	145.0
79.10	120.0
81.00	118.0
82.00	108.0
83.10	157.0
84.10	125.0
84.90	159.0
95.90	112.0
97.00	167.0
98.00	190.0
105.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	620.0
37.00	3003.0
38.00	2858.0
39.00	1120.0
39.90	248.0
41.00	496.0
42.10	262.0
43.00	507.0
44.00	2903.0
45.00	785.0
45.90	126.0
47.00	627.0
48.00	351.0
49.00	2708.0
50.00	11879.0
51.00	3561.0
51.90	203.0
53.00	128.0
55.00	499.0
56.10	1049.0
57.00	1948.0
58.00	184.0
60.00	708.0
61.00	2756.0
62.00	2912.0
63.00	2113.0
64.10	206.0
68.00	6175.0
69.00	6458.0
70.10	604.0
71.00	249.0
72.00	393.0
73.00	2794.0
74.00	10174.0
75.00	29544.0
76.10	2613.0
77.00	549.0
78.00	321.0
78.90	1913.0
80.00	618.0
80.90	2073.0
81.90	455.0
83.00	157.0
86.00	144.0
87.00	2254.0
88.00	2048.0
90.90	346.0
92.00	1674.0
93.00	2366.0
94.00	7202.0
95.00	55728.0
96.10	3669.0
97.00	222.0
98.10	137.0
103.80	301.0
105.20	174.0
105.90	288.0
107.00	129.0
109.00	105.0
111.00	122.0
115.80	225.0
116.90	425.0
117.90	212.0
118.90	295.0
127.90	221.0
129.00	146.0
129.80	176.0
131.00	139.0
134.80	122.0
137.00	169.0
140.90	549.0
142.90	582.0
147.90	113.0
154.90	176.0
174.00	37504.0
175.00	3072.0
176.00	35960.0
177.00	2547.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	605.0
37.00	3144.0
38.00	2857.0
39.00	1258.0
39.90	250.0
41.00	554.0
42.00	250.0
43.10	527.0
44.00	2927.0
45.00	847.0
45.80	122.0
47.10	699.0
48.00	397.0
49.00	2866.0
50.00	13020.0
51.00	3793.0
51.90	184.0
52.90	102.0
55.10	490.0
56.00	1134.0
57.00	2052.0
58.00	205.0
60.00	770.0
61.00	3009.0
62.00	3088.0
63.00	2167.0
64.00	261.0
67.00	292.0
68.00	6698.0
69.00	6847.0
70.00	588.0
71.00	239.0
72.00	388.0
73.00	3147.0
74.00	11219.0
75.00	32136.0
76.10	2884.0
77.00	590.0
78.00	335.0
79.00	2081.0
80.00	573.0
80.90	2183.0
82.00	495.0
83.00	175.0
86.00	106.0
87.00	2418.0
88.00	2200.0
90.90	390.0
92.00	1828.0
93.00	2687.0
94.00	7710.0
95.00	61184.0
96.00	3942.0
97.00	265.0
98.00	140.0
103.80	341.0
105.10	172.0
106.00	313.0
107.00	129.0
111.00	110.0
114.80	110.0
115.80	268.0
116.90	444.0
117.90	222.0
118.90	358.0
127.90	254.0
129.00	182.0
129.80	225.0
131.00	157.0
134.80	113.0
137.00	147.0
141.00	608.0
142.90	635.0
147.80	126.0
154.90	174.0
174.00	41856.0
175.00	3359.0
176.00	40488.0
177.00	2835.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	582.0
37.00	3028.0
38.00	2613.0
39.00	1318.0
39.90	272.0
41.00	592.0
42.00	236.0
43.10	541.0
44.00	2870.0
45.00	775.0
45.80	112.0
47.10	711.0
48.00	422.0
49.00	2746.0
50.00	12516.0
51.00	3687.0
52.00	195.0
55.10	539.0
56.00	1152.0
57.00	1928.0
58.00	220.0
60.00	790.0
61.00	2973.0
62.00	3015.0
63.00	2094.0
64.00	291.0
67.00	321.0
68.00	6476.0
69.00	6536.0
70.00	542.0
71.00	213.0
71.90	364.0
73.00	3113.0
74.00	10959.0
75.00	31760.0
76.10	2827.0
77.00	504.0
78.00	318.0
79.00	2085.0
79.90	479.0
80.90	2022.0
82.00	516.0
83.00	189.0
85.10	115.0
87.00	2358.0
88.00	2237.0
91.00	394.0
92.00	1822.0
93.00	2748.0
94.10	7495.0
95.00	60864.0
96.00	3892.0
97.00	253.0
98.00	153.0
103.80	342.0
105.00	180.0
106.00	319.0
107.00	117.0
111.00	113.0
114.80	140.0
115.80	266.0
116.90	432.0
117.90	224.0
118.90	376.0
127.90	241.0
128.90	198.0
129.80	256.0
131.00	162.0
134.90	114.0
136.90	115.0
141.00	612.0
142.90	614.0
145.80	106.0
147.80	130.0
154.90	164.0
158.90	115.0
174.00	42664.0
175.00	3362.0
176.00	41224.0
177.00	2796.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205