




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082418\
Data File : VV007178.D
Acq On : 24 Aug 2018 19:23
Operator : SY/MD
Sample : J4599-19DL 20X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBM1DL

Manual Integrations
APPROVED

MMDadoda
8/25/2018 9:54:10 AM

Quant Time: Aug 25 00:15:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 25 00:12:31 2018
Response via : Initial Calibration

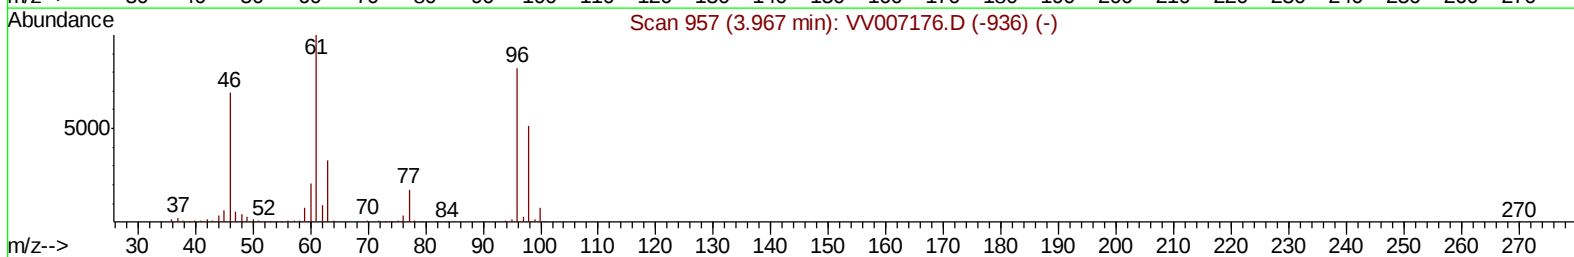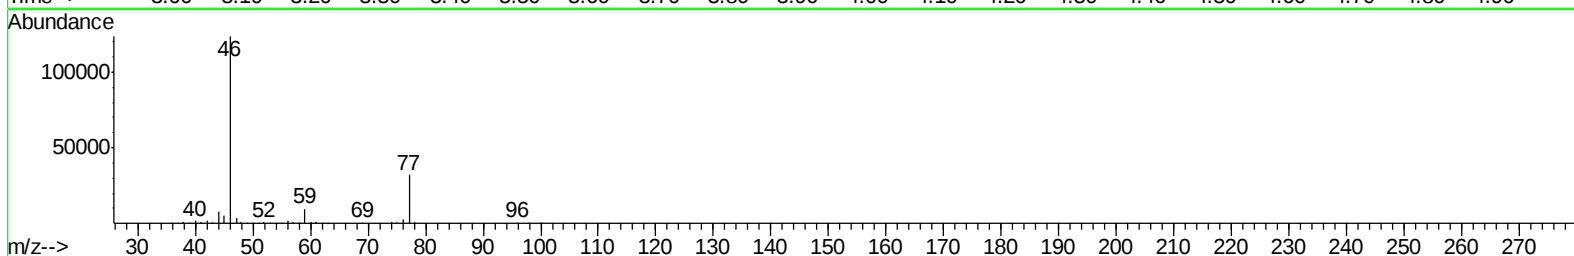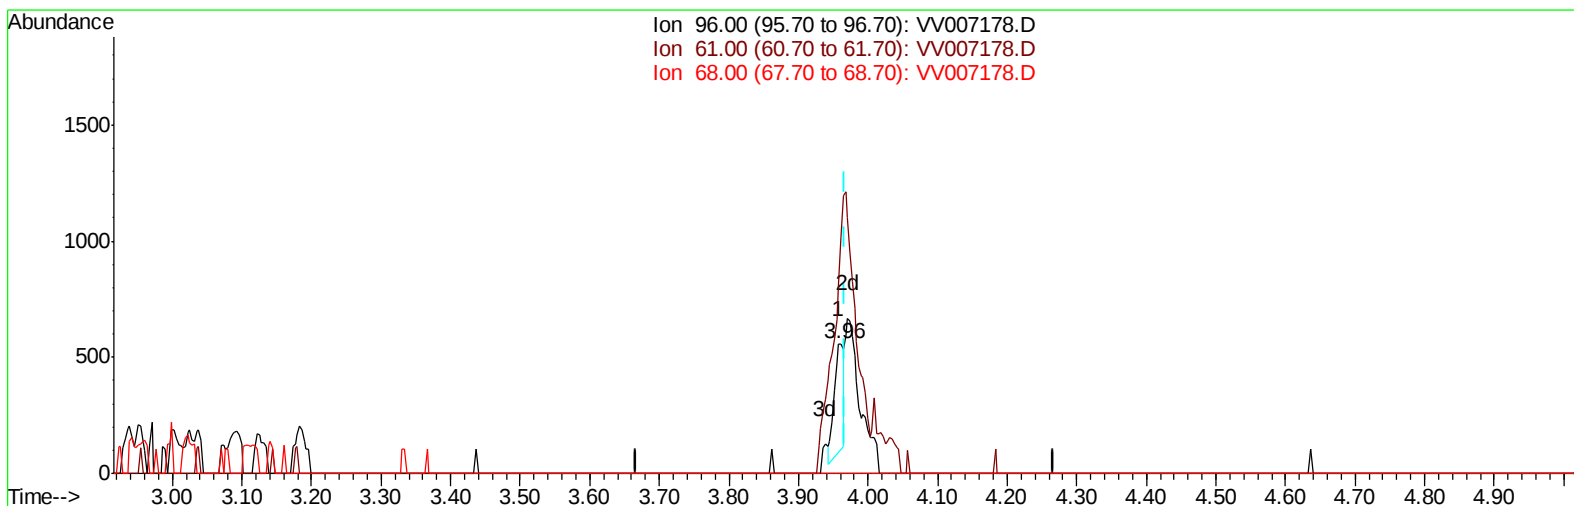

TIC: VV007178.D

(20) cis-1,2-Dichloroethene (T)

3.958min (-0.010) 0.09ug/L

response 444

Ion	Exp%	Act%
96.00	100	100
61.00	126.00	143.99
68.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082418\
Data File : VV007178.D
Acq On : 24 Aug 2018 19:23
Operator : SY/MD
Sample : J4599-19DL 20X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBM1DL

Manual Integrations
APPROVED

MMDadoda
8/25/2018 9:54:10 AM

Quant Time: Aug 25 00:15:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 25 00:12:31 2018
Response via : Initial Calibration

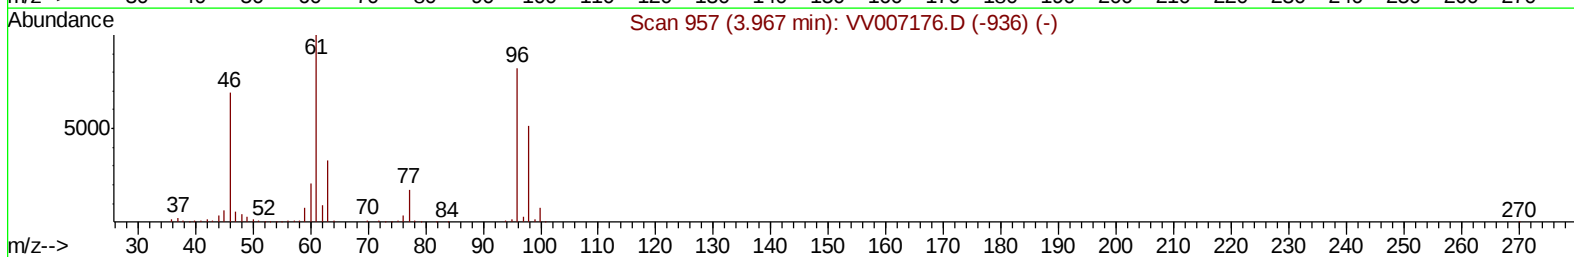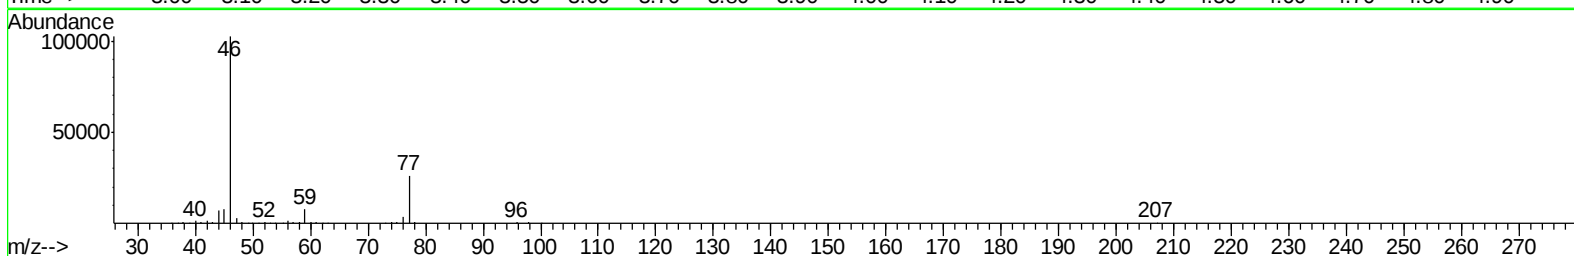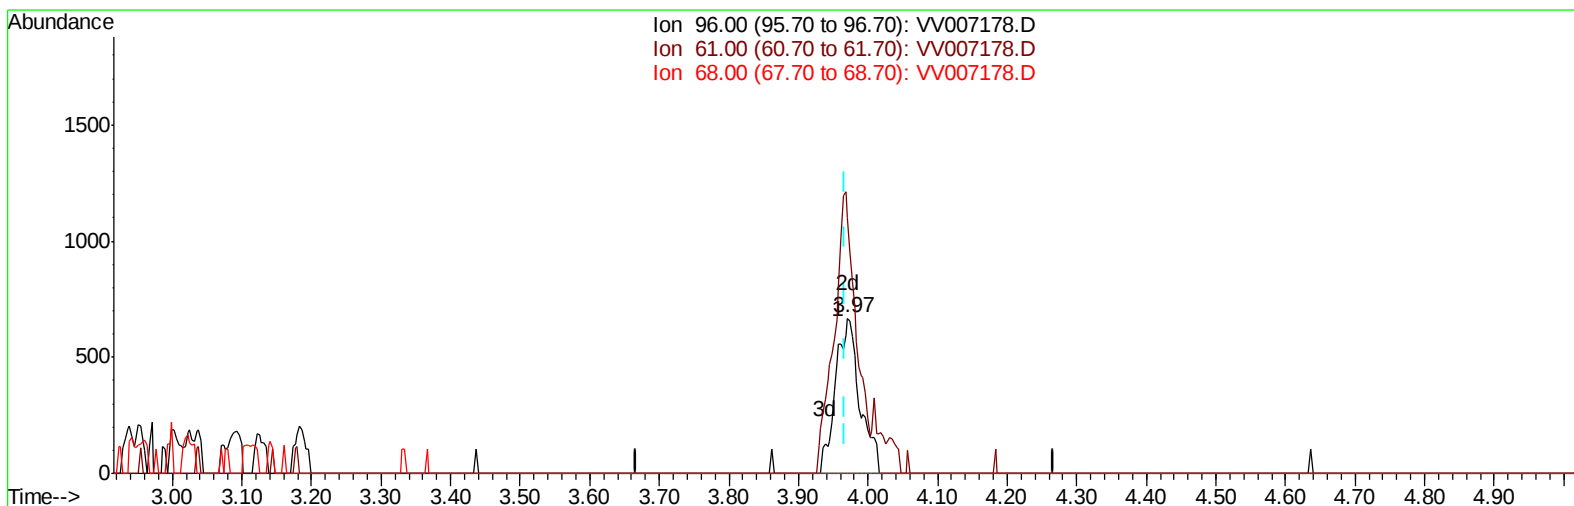

TIC: VV007178.D

(20) cis-1,2-Dichloroethene (T)

3.971min (+0.003) 0.32ug/L m

response 1622

Ion	Exp%	Act%
96.00	100	100
61.00	126.00	164.92#
68.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082418\
 Data File : VV007178.D
 Acq On : 24 Aug 2018 19:23
 Operator : SY/MD
 Sample : J4599-19DL 20X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBM1DL

Manual Integrations
 APPROVED

MMDadoda
 8/25/2018 9:54:10 AM

Quant Time: Aug 25 00:28:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 25 00:12:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	655102	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	637786	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	256058	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	214442	46.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.20%
7) Chloroethane-d5	1.58	69	177319	47.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.04%
11) 1,1-Dichloroethene-d2	2.13	63	286494	35.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.58%
21) 2-Butanone-d5	3.96	46	333639	97.29	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.29%
24) Chloroform-d	4.41	84	415421	46.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.02%
26) 1,2-Dichloroethane-d4	5.09	65	266103	49.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.54%
32) Benzene-d6	5.11	84	860781	47.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.02%
36) 1,2-Dichloropropane-d6	6.12	67	284487	47.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.70%
41) Toluene-d8	7.37	98	699534	43.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.72%
43) trans-1,3-Dichloropropene-	7.67	79	113339	43.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.24%
47) 2-Hexanone-d5	8.14	63	149868	79.89	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.89%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	366760	46.31	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.62%
64) 1,2-Dichlorobenzene-d4	11.68	152	263521	49.31	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.62%

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082418\
Data File : VV007178.D
Acq On : 24 Aug 2018 19:23
Operator : SY/MD
Sample : J4599-19DL 20X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBM1DL

Manual Integrations
APPROVED

MMDadoda
8/25/2018 9:54:10 AM

Quant Time: Aug 25 00:28:16 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 25 00:12:31 2018
Response via : Initial Calibration

