

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
 Data File : VV007186.D
 Acq On : 24 Aug 2018 22:41
 Operator : SY/MD
 Sample : J4622-18DL 200X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBL0DL

Quant Time: Aug 25 01:11:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 25 00:12:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	630854	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	619456	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	249502	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	215938	48.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.46%
7) Chloroethane-d5	1.58	69	179253	49.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.78%
11) 1,1-Dichloroethene-d2	2.13	63	285953	37.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.18%
21) 2-Butanone-d5	3.96	46	331532	100.39	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.39%
24) Chloroform-d	4.41	84	427065	49.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.30%
26) 1,2-Dichloroethane-d4	5.09	65	267468	51.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.84%
32) Benzene-d6	5.11	84	863105	49.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.10%
36) 1,2-Dichloropropane-d6	6.12	67	285286	49.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.80%
41) Toluene-d8	7.37	98	685040	44.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.44%
43) trans-1,3-Dichloropropene-	7.67	79	113722	45.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.12%
47) 2-Hexanone-d5	8.14	63	142879	78.42	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.42%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	371688	48.32	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.64%
64) 1,2-Dichlorobenzene-d4	11.68	152	265068	50.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Qvalue
5) Vinyl chloride	1.32	62	400588	75.525 ug/L	99
20) cis-1,2-Dichloroethene	3.97	96	267005	54.245 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
Data File : VV007186.D
Acq On : 24 Aug 2018 22:41
Operator : SY/MD
Sample : J4622-18DL 200X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBL0DL

Quant Time: Aug 25 01:11:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 25 00:12:31 2018
Response via : Initial Calibration

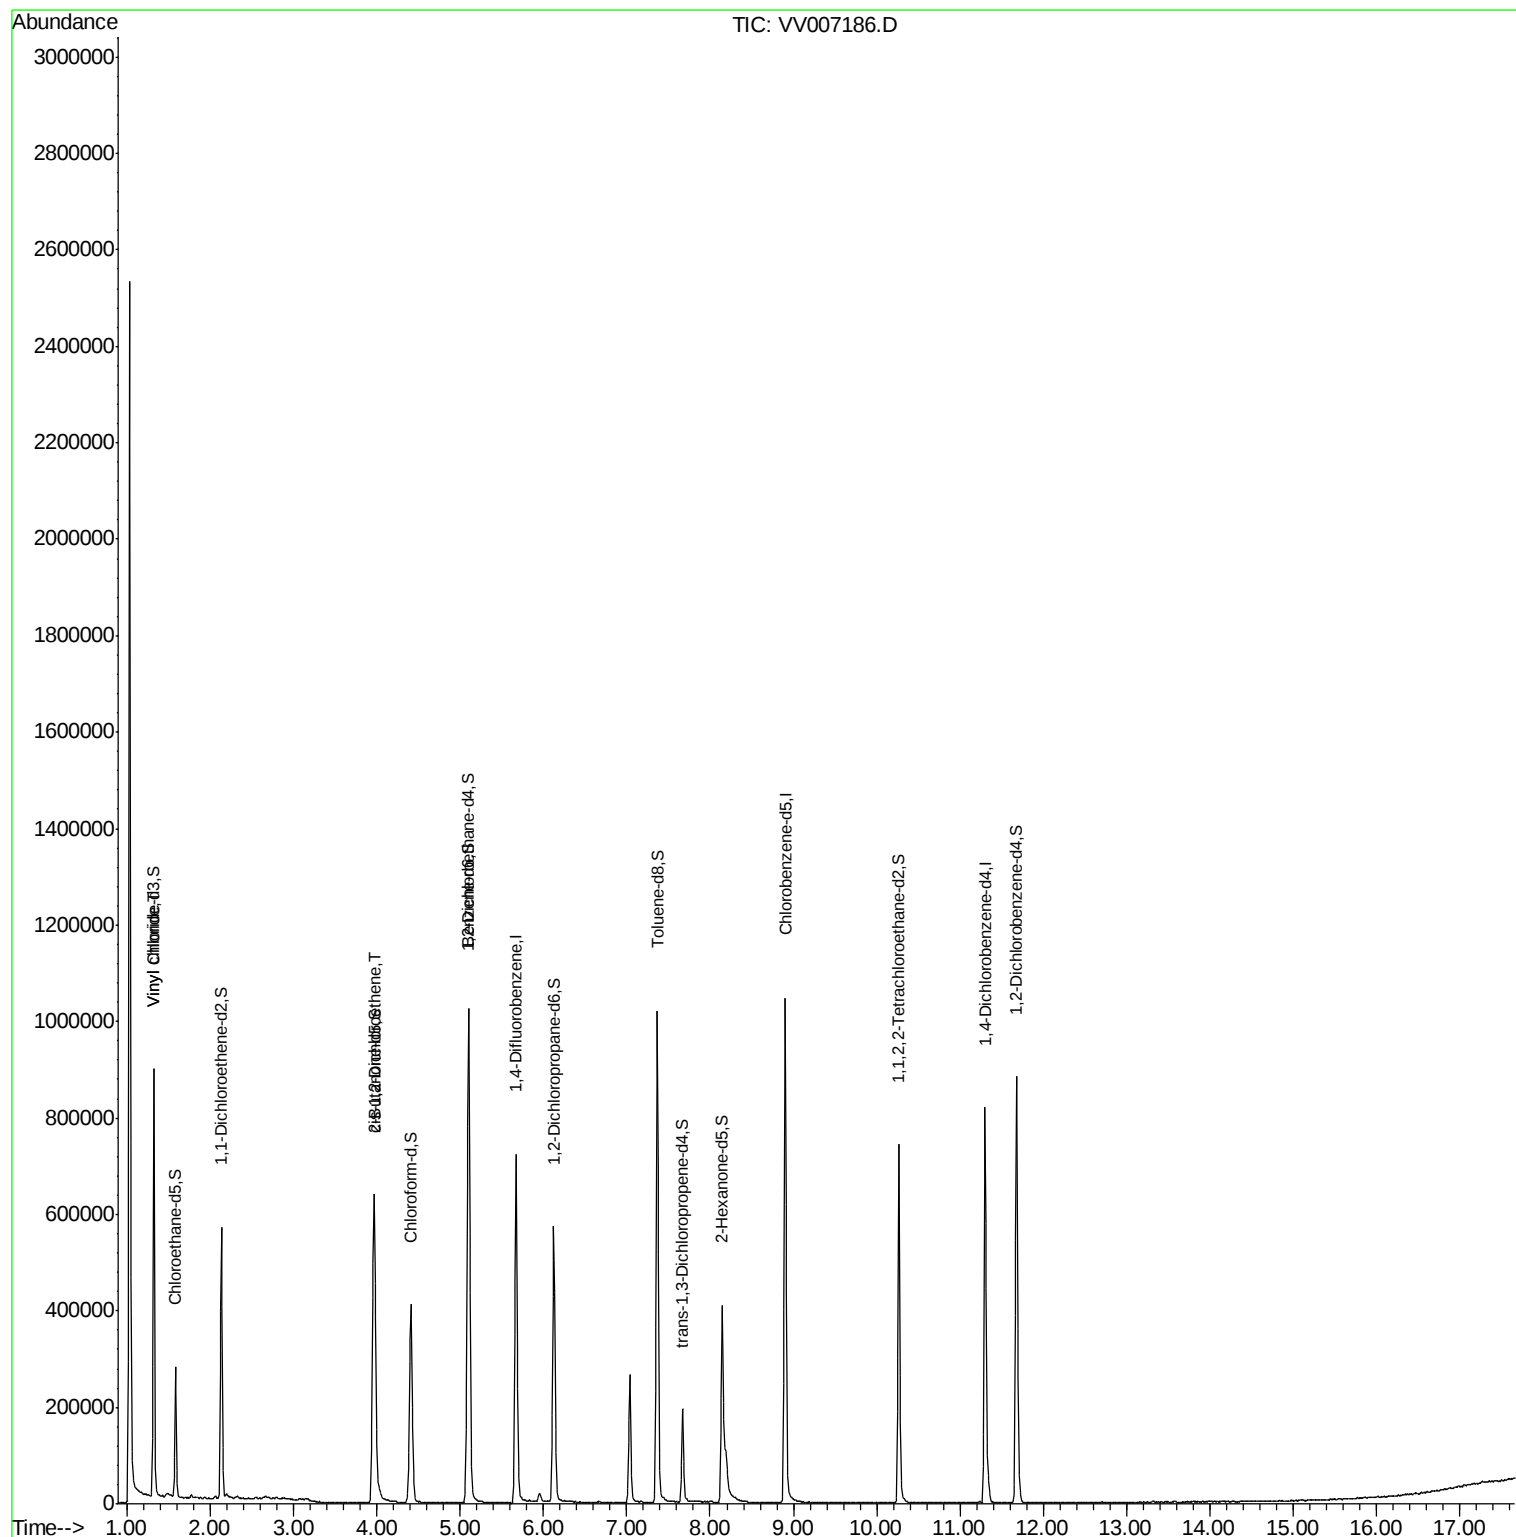

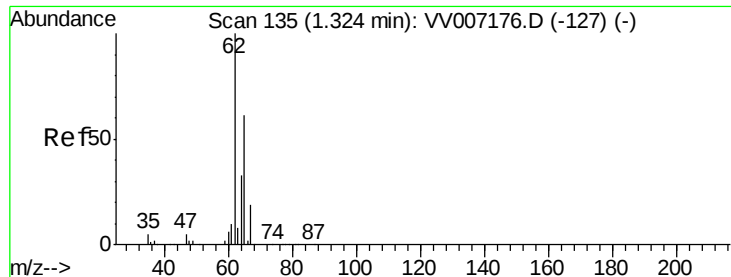

#5

Vinyl chloride

Concen: 75.525 ug/L

RT: 1.32 min Scan# 135

Delta R.T. 0.00 min

Lab File: VV007186.D

Acq: 24 Aug 2018 22:41

Instrument :

MSVOA_V

ClientSampleId :


ETBL0DL

Tgt Ion: 62 Resp: 400588

Ion Ratio Lower Upper

62 100

64 32.2 22.9 42.5

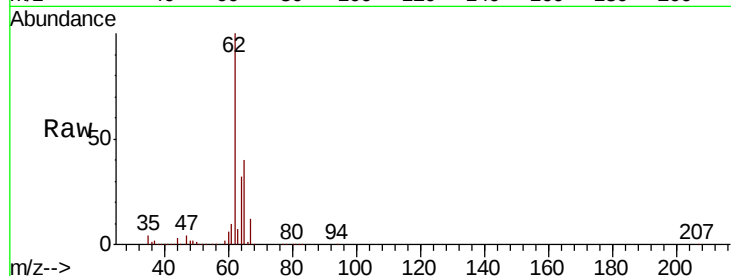

Abundance Ion 62.00 (61.70 to 62.70): VV007176.D (-127) (-)

Ion 64.00 (63.70 to 64.70): VV007176.D (-127) (-)

1.32

400000

300000



200000

100000

0

1.30 1.40

Time-->

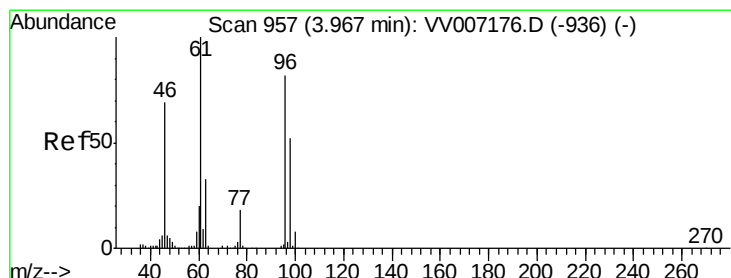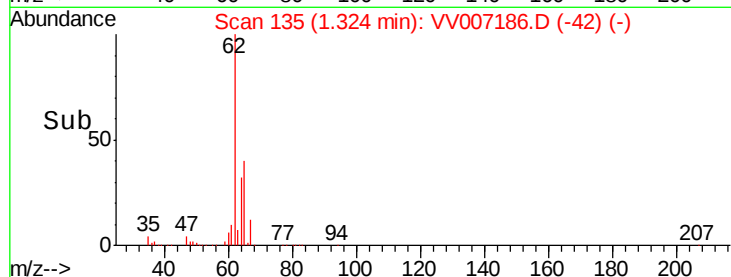

#20

cis-1,2-Dichloroethene

Concen: 54.245 ug/L

RT: 3.97 min Scan# 957

Delta R.T. 0.00 min

Lab File: VV007186.D

Acq: 24 Aug 2018 22:41


Tgt Ion: 96 Resp: 267005

Ion Ratio Lower Upper

96 100

61 124.9 88.2 163.8

68 0.0 0.0 0.0

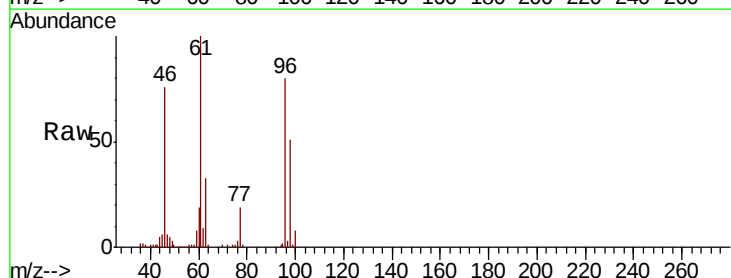

Abundance Ion 96.00 (95.70 to 96.70): VV007176.D (-936) (-)

Ion 61.00 (60.70 to 61.70): VV007176.D (-936) (-)

Ion 68.00 (67.70 to 68.70): VV007176.D (-936) (-)

150000

100000

50000

0

3.85 3.90 3.95 4.00 4.05

Time-->

