

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
 Data File : VV007187.D
 Acq On : 24 Aug 2018 23:06
 Operator : SY/MD
 Sample : J4622-19RE
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBL1RE

Quant Time: Aug 25 01:20:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 25 00:12:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	639474	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	637561	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	261297	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	210329	46.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.64%
7) Chloroethane-d5	1.58	69	179314	49.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.46%
11) 1,1-Dichloroethene-d2	2.13	63	292335	37.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.82%
21) 2-Butanone-d5	3.96	46	324467	96.93	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.93%
24) Chloroform-d	4.41	84	427287	49.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.02%
26) 1,2-Dichloroethane-d4	5.09	65	270221	51.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.50%
32) Benzene-d6	5.11	84	865701	47.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.12	67	288699	48.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.14%
41) Toluene-d8	7.37	98	704846	44.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.40%
43) trans-1,3-Dichloropropene-	7.67	79	109814	42.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.56%
47) 2-Hexanone-d5	8.14	63	137434	73.29	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	73.29%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	374804	47.34	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.68%
64) 1,2-Dichlorobenzene-d4	11.68	152	270476	49.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.20%


Target Compounds					Qvalue
13) Acetone	2.20	43	8023	3.246 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
Data File : VV007187.D
Acq On : 24 Aug 2018 23:06
Operator : SY/MD
Sample : J4622-19RE
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBL1RE

Quant Time: Aug 25 01:20:26 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 25 00:12:31 2018
Response via : Initial Calibration

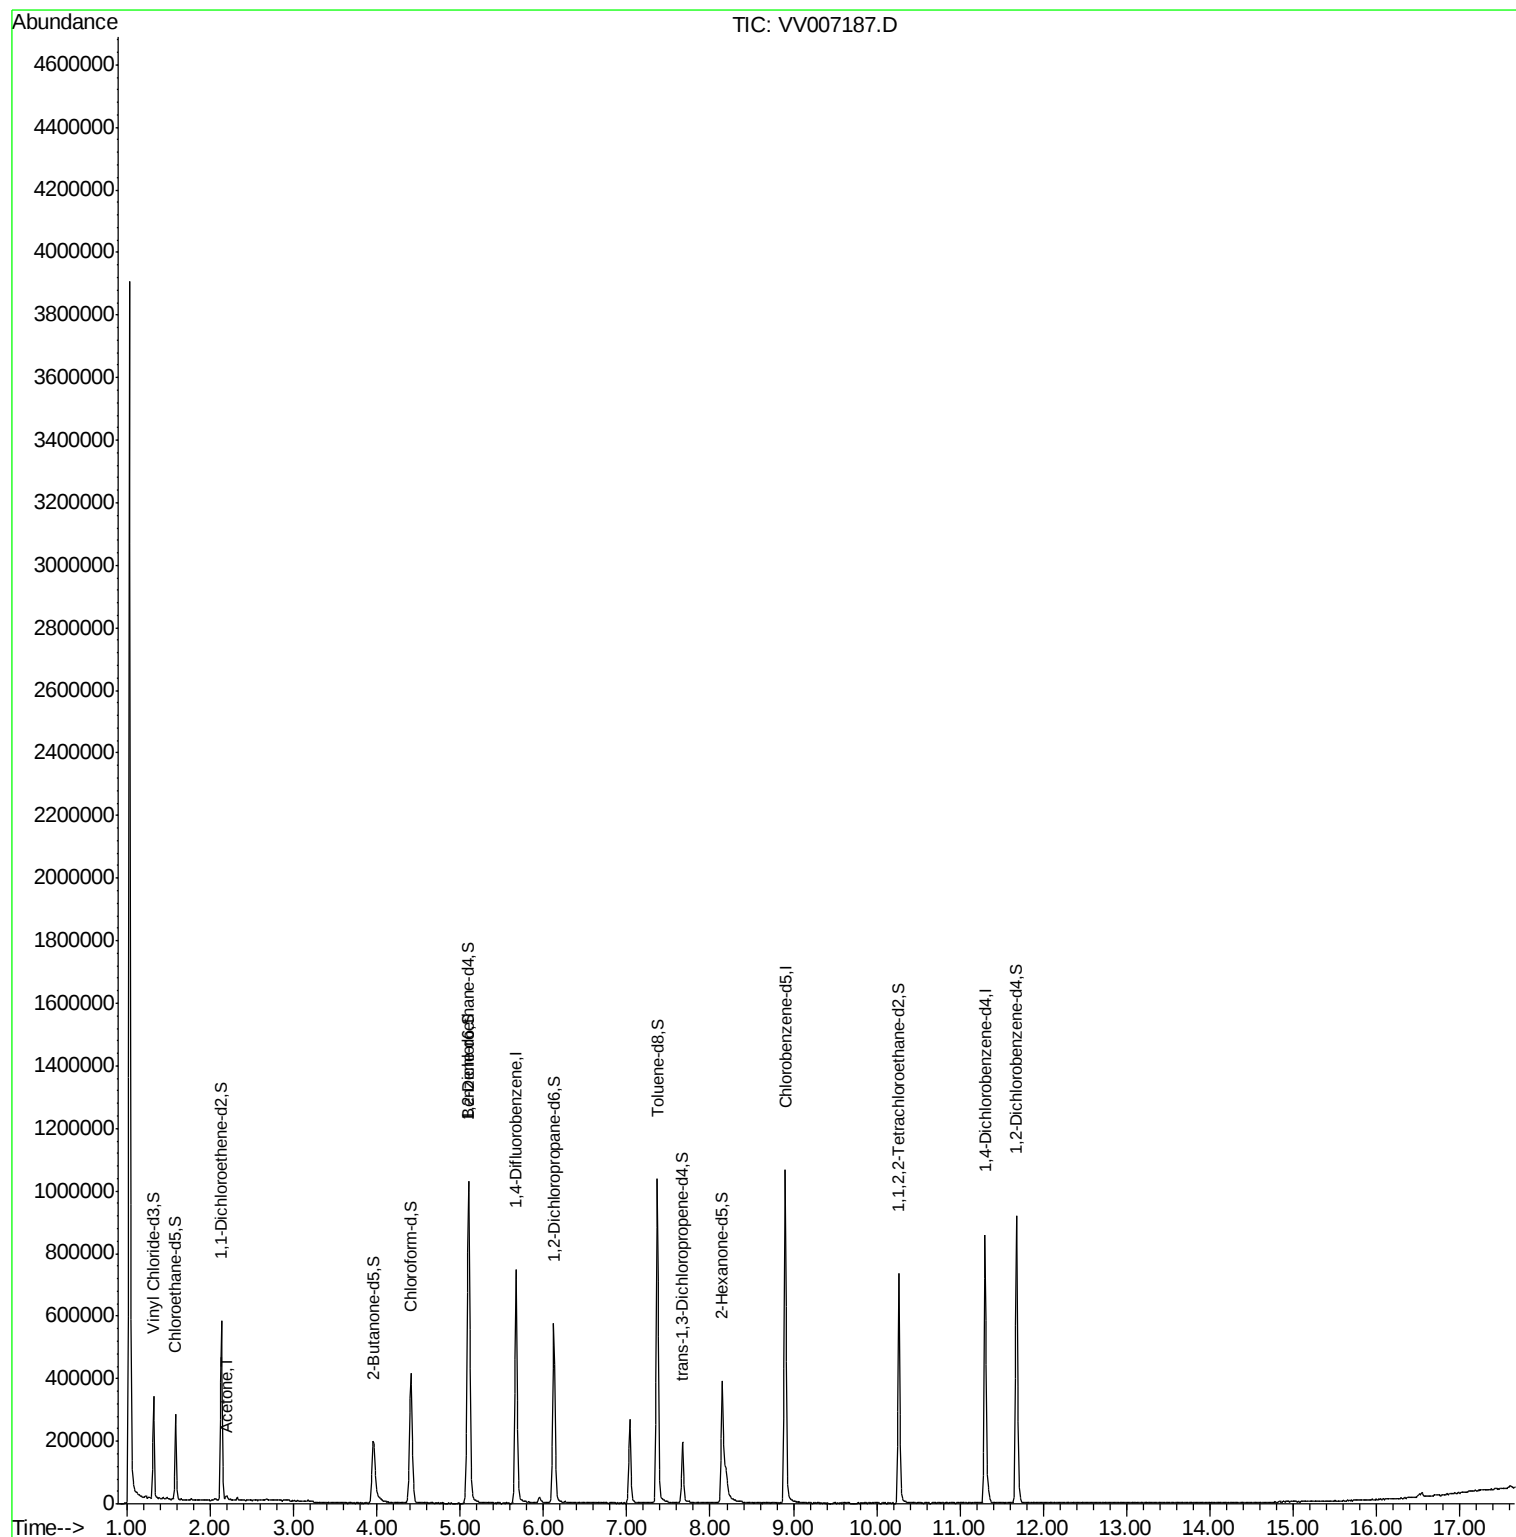

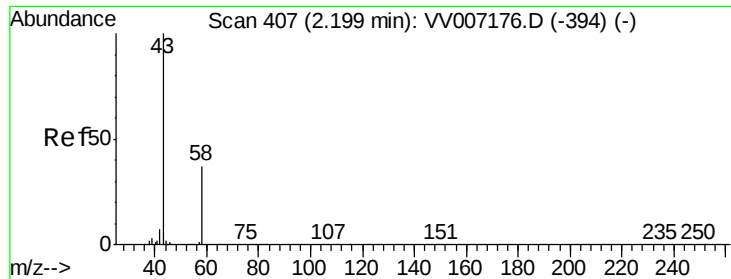

#13

Acetone

Concen: 3.246 ug/L

RT: 2.20 min Scan# 407

Delta R.T. 0.00 min

Lab File: VV007187.D

Acq: 24 Aug 2018 23:06

Instrument :
MSVOA_V
ClientSampleId :
ETBL1RE

Tgt Ion: 43 Resp: 8023

Ion Ratio Lower Upper

43 100

58 32.2 0.0 72.0

