

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
 Data File : VV007185.D
 Acq On : 24 Aug 2018 22:16
 Operator : SY/MD
 Sample : J4622-17DL 20X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.916	5	8	14	rBV4	605	606	0.02%	0.003%
2	1.029	30	43	66	rBV	2432733	3192424	100.00%	14.054%
3	1.321	125	134	157	rVB2	673894	754072	23.62%	3.320%
4	1.582	208	215	229	rVB	261314	304921	9.55%	1.342%
5	2.132	376	386	399	rBV	553616	793715	24.86%	3.494%
6	3.292	745	747	752	rVB5	1527	1058	0.03%	0.005%
7	3.318	752	755	758	rBV3	1008	672	0.02%	0.003%
8	3.627	848	851	854	rBV4	572	499	0.02%	0.002%
9	3.739	881	886	888	rBV3	851	873	0.03%	0.004%
10	3.787	897	901	909	rBV5	825	991	0.03%	0.004%
11	3.871	923	927	931	rVB4	729	543	0.02%	0.002%
12	3.967	937	957	1004	rBV2	740433	1973282	61.81%	8.687%
13	4.408	1075	1094	1122	rBV	404072	967108	30.29%	4.257%
14	4.594	1150	1152	1155	rBV3	822	484	0.02%	0.002%
15	4.633	1162	1164	1168	rVB	714	406	0.01%	0.002%
16	4.656	1168	1171	1175	rBV3	857	686	0.02%	0.003%
17	4.675	1175	1177	1181	rBV4	643	428	0.01%	0.002%
18	4.733	1193	1195	1199	rVB4	802	406	0.01%	0.002%
19	4.755	1199	1202	1206	rBV3	673	590	0.02%	0.003%
20	4.829	1222	1225	1229	rVB4	905	637	0.02%	0.003%
21	4.884	1240	1242	1250	rVB4	605	487	0.02%	0.002%
22	5.099	1289	1309	1341	rBV2	1016698	2433553	76.23%	10.713%
23	5.395	1397	1401	1403	rBV2	684	580	0.02%	0.003%
24	5.411	1403	1406	1411	rVB3	731	523	0.02%	0.002%
25	5.443	1411	1416	1419	rBV5	1427	1249	0.04%	0.005%
26	5.508	1433	1436	1439	rVB3	854	532	0.02%	0.002%
27	5.527	1439	1442	1444	rBV3	733	420	0.01%	0.002%
28	5.598	1461	1464	1469	rBV4	808	700	0.02%	0.003%
29	5.672	1469	1487	1514	rBV	721230	1444432	45.25%	6.359%
30	5.964	1564	1578	1593	rBV2	207248	409513	12.83%	1.803%
31	6.125	1614	1628	1653	rBV	555107	1112667	34.85%	4.898%
32	6.684	1799	1802	1806	rVB3	992	679	0.02%	0.003%
33	6.752	1820	1823	1828	rVB4	1297	935	0.03%	0.004%
34	6.848	1849	1853	1859	rVB6	1062	1102	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
 Data File : VV007185.D
 Acq On : 24 Aug 2018 22:16
 Operator : SY/MD
 Sample : J4622-17DL 20X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Title : VOC Analysis

35	6.884	1859	1864	1867	rBV4	1277	944	0.03%	0.004%
36	6.942	1878	1882	1886	rBV5	696	698	0.02%	0.003%
37	7.035	1897	1911	1932	rBV	260238	478040	14.97%	2.104%
38	7.366	2000	2014	2037	rBV	1015544	1774992	55.60%	7.814%
39	7.668	2096	2108	2126	rBV	188303	326207	10.22%	1.436%
40	7.803	2147	2150	2154	rBV5	1476	1261	0.04%	0.006%
41	8.144	2243	2256	2266	rBV	392755	775764	24.30%	3.415%
42	8.536	2375	2378	2380	rBV3	645	469	0.01%	0.002%
43	8.607	2398	2400	2403	rVB3	831	405	0.01%	0.002%
44	8.694	2424	2427	2429	rBV4	624	425	0.01%	0.002%
45	8.742	2437	2442	2446	rVB4	705	758	0.02%	0.003%
46	8.819	2462	2466	2471	rBV4	1060	1181	0.04%	0.005%
47	8.903	2478	2492	2517	rBV	1060199	1772836	55.53%	7.804%
48	9.189	2577	2581	2589	rVB7	2249	2868	0.09%	0.013%
49	9.224	2589	2592	2595	rVB2	837	562	0.02%	0.002%
50	9.263	2602	2604	2608	rVB3	684	389	0.01%	0.002%
51	9.289	2608	2612	2616	rVB5	641	617	0.02%	0.003%
52	9.366	2633	2636	2639	rBV2	730	508	0.02%	0.002%
53	9.456	2660	2664	2666	rBV4	665	397	0.01%	0.002%
54	9.507	2677	2680	2685	rBV6	713	653	0.02%	0.003%
55	9.540	2688	2690	2693	rVB3	698	474	0.01%	0.002%
56	9.559	2693	2696	2699	rBV3	794	478	0.01%	0.002%
57	9.601	2703	2709	2710	rBV2	1439	1423	0.04%	0.006%
58	9.675	2728	2732	2734	rBV2	511	406	0.01%	0.002%
59	9.752	2752	2756	2761	rBV6	778	736	0.02%	0.003%
60	9.781	2761	2765	2768	rVB3	730	461	0.01%	0.002%
61	9.842	2780	2784	2787	rBV4	711	506	0.02%	0.002%
62	9.864	2789	2791	2794	rVB	833	361	0.01%	0.002%
63	9.896	2794	2801	2804	rBV3	791	904	0.03%	0.004%
64	9.922	2804	2809	2812	rVB3	789	701	0.02%	0.003%
65	9.945	2812	2816	2818	rBV3	556	429	0.01%	0.002%
66	9.974	2823	2825	2827	rBV3	740	424	0.01%	0.002%
67	10.099	2861	2864	2867	rVB3	745	471	0.01%	0.002%
68	10.208	2893	2898	2902	rVB5	776	678	0.02%	0.003%
69	10.266	2902	2916	2935	rBV	715108	1156582	36.23%	5.092%
70	10.427	2962	2966	2969	rBV3	515	403	0.01%	0.002%
71	10.446	2969	2972	2976	rBV3	673	408	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
 Data File : VV007185.D
 Acq On : 24 Aug 2018 22:16
 Operator : SY/MD
 Sample : J4622-17DL 20X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Title : VOC Analysis

72	10.469	2976	2979	2982	rBV4	770	601	0.02%	0.003%
73	10.523	2990	2996	2998	rBV5	1016	1210	0.04%	0.005%
74	10.630	3026	3029	3034	rVB4	738	589	0.02%	0.003%
75	10.659	3035	3038	3040	rBV	648	357	0.01%	0.002%
76	10.697	3047	3050	3053	rVB3	757	468	0.01%	0.002%
77	10.761	3066	3070	3073	rVV2	738	581	0.02%	0.003%
78	10.800	3080	3082	3087	rVB3	1076	760	0.02%	0.003%
79	10.903	3111	3114	3118	rVV4	1143	1034	0.03%	0.005%
80	10.935	3122	3124	3129	rVB4	902	758	0.02%	0.003%
81	10.958	3129	3131	3133	rBV2	758	460	0.01%	0.002%
82	10.974	3133	3136	3139	rBV5	605	556	0.02%	0.002%
83	11.105	3174	3177	3182	rBV3	837	631	0.02%	0.003%
84	11.234	3210	3217	3218	rBV3	2108	2200	0.07%	0.010%
85	11.302	3225	3238	3263	rBV	812580	1451744	45.47%	6.391%
86	11.488	3293	3296	3299	rBV3	616	370	0.01%	0.002%
87	11.533	3308	3310	3312	rBV3	633	393	0.01%	0.002%
88	11.678	3340	3355	3377	rBV	879645	1535670	48.10%	6.760%
89	11.906	3420	3426	3430	rBV6	988	1168	0.04%	0.005%
90	11.957	3438	3442	3448	rVV4	754	857	0.03%	0.004%
91	12.115	3488	3491	3495	rBV3	933	800	0.03%	0.004%
92	12.144	3498	3500	3505	rVB3	629	397	0.01%	0.002%
93	12.372	3569	3571	3574	rVB3	921	505	0.02%	0.002%
94	12.395	3574	3578	3579	rBV4	832	530	0.02%	0.002%
95	12.536	3620	3622	3625	rVB2	1027	465	0.01%	0.002%
96	12.697	3669	3672	3675	rBV3	1341	1173	0.04%	0.005%
97	12.871	3722	3726	3728	rBV	541	448	0.01%	0.002%
98	12.932	3742	3745	3749	rVB5	1320	1025	0.03%	0.005%
99	13.494	3916	3920	3922	rBV5	1258	930	0.03%	0.004%
100	13.887	4038	4042	4047	rBV6	1491	1540	0.05%	0.007%


Sum of corrected areas: 22715812

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
Data File : VV007185.D
Acq On : 24 Aug 2018 22:16
Operator : SY/MD
Sample : J4622-17DL 20X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBK9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

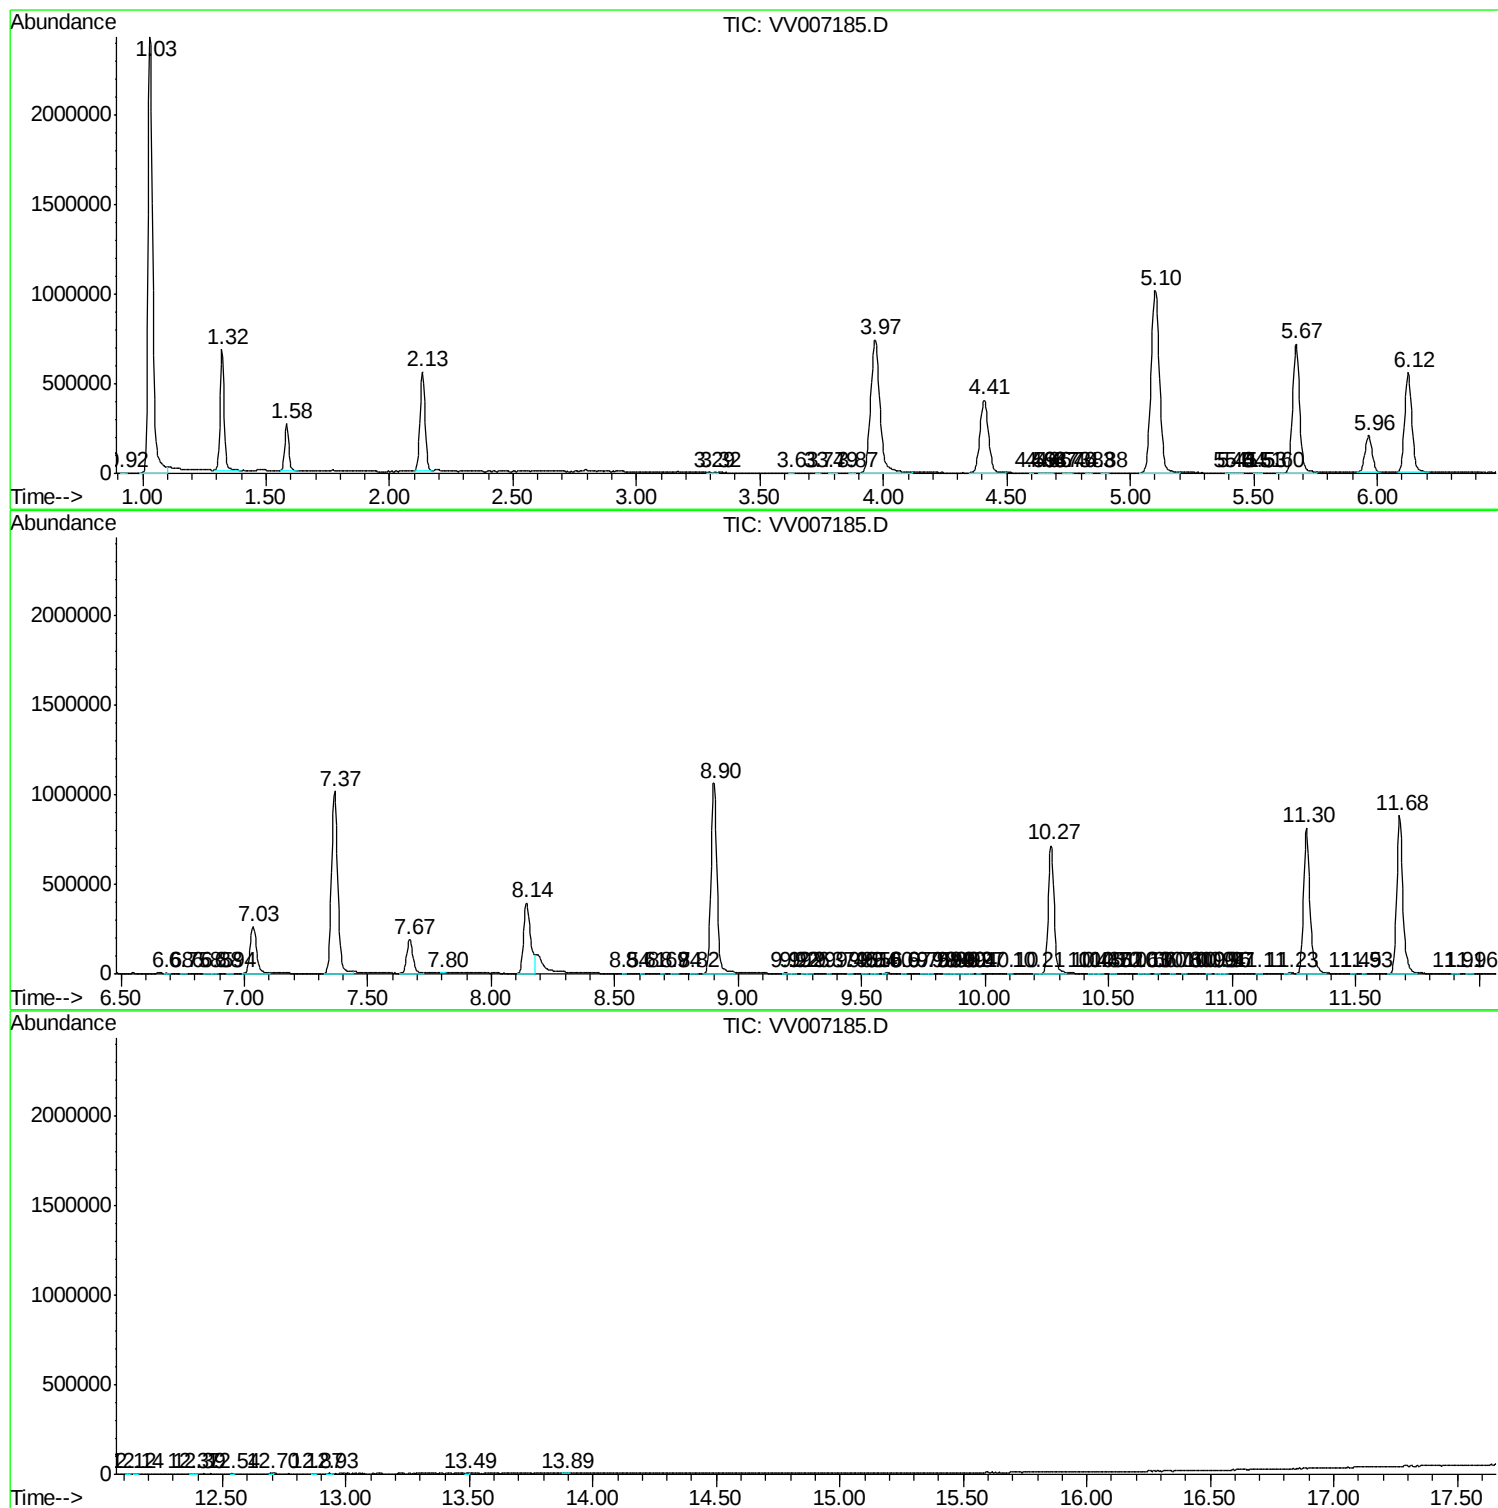

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
Data File : VV007185.D
Acq On : 24 Aug 2018 22:16
Operator : SY/MD
Sample : J4622-17DL 20X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBK9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082418\
Data File : VV007185.D
Acq On : 24 Aug 2018 22:16
Operator : SY/MD
Sample : J4622-17DL 20X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBK9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc