


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082418\
 Data File : VV007167.D
 Acq On : 24 Aug 2018 12:47
 Operator : SY/MD
 Sample : BFB64
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 27 01:23:53 2018

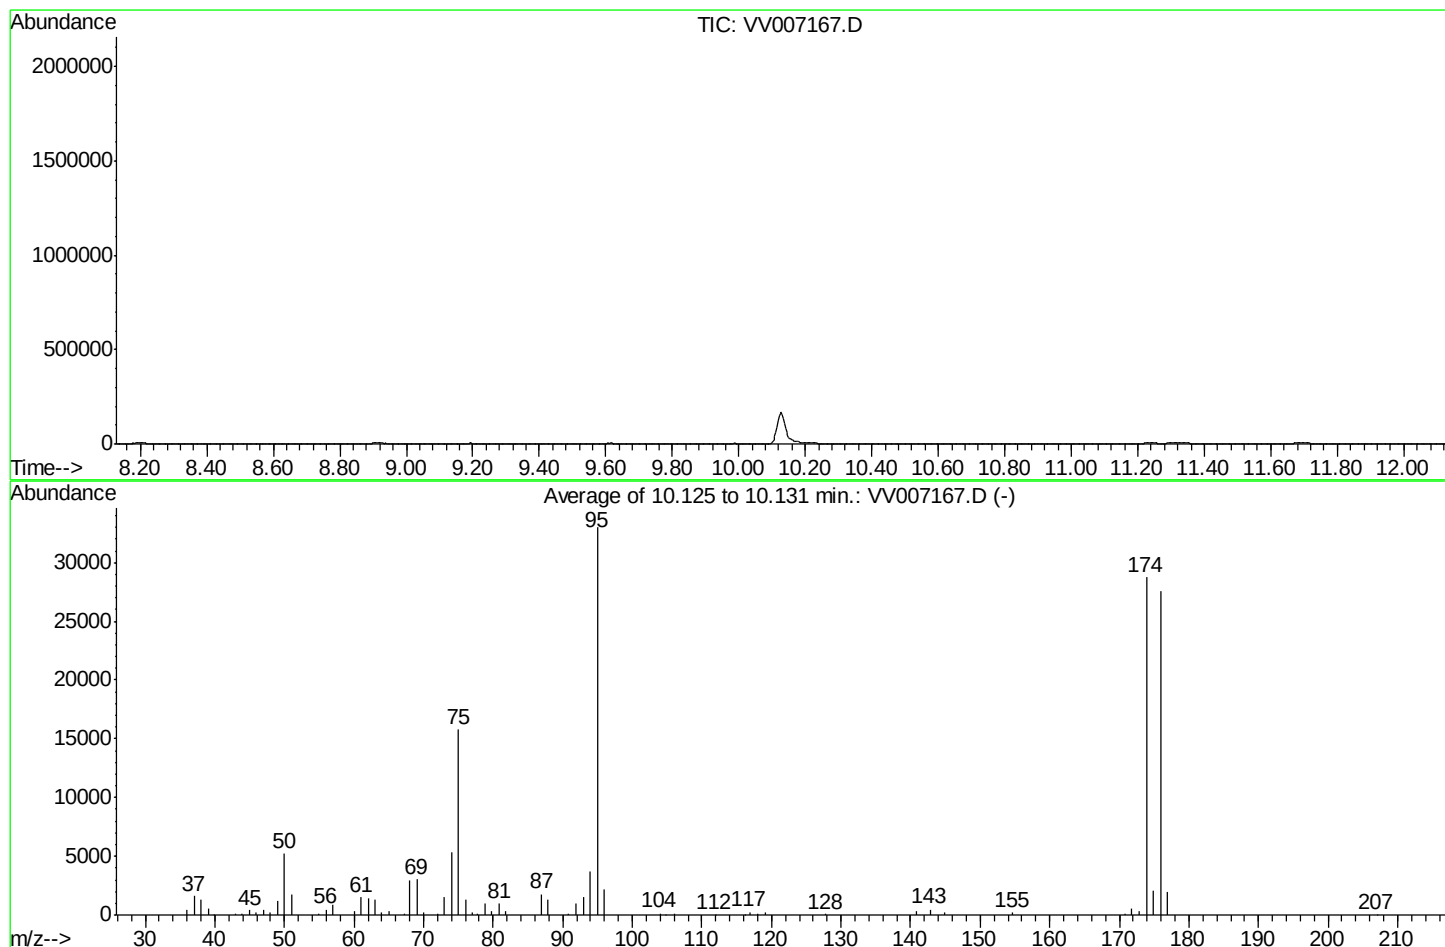

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2861

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	5196	PASS
75	95	30	80	47.8	15769	PASS
95	95	100	100	100.0	33002	PASS
96	95	5	9	6.6	2173	PASS
173	174	0.00	2	1.3	361	PASS
174	95	50	120	87.0	28725	PASS
175	174	5	9	7.3	2106	PASS
176	174	95	101	95.9	27552	PASS
177	176	5	9	7.1	1967	PASS

Scan 2861 (10.089 min): VV007167.D
BFB64

m/z	Abundance
39.90	474.0
43.90	1164.0
73.30	115.0
207.10	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	386.0
37.00	1817.0
38.00	1267.0
39.10	597.0
39.90	491.0
43.90	1332.0
45.00	314.0
45.90	155.0
47.10	444.0
48.00	170.0
49.00	1284.0
50.00	5336.0
51.00	1798.0
55.00	128.0
56.00	481.0
56.90	1038.0
60.00	363.0
61.00	1315.0
62.00	1491.0
63.00	1392.0
63.90	231.0
64.90	290.0
67.20	110.0
67.90	3075.0
69.00	2950.0
70.00	265.0
71.90	173.0
73.00	1525.0
74.00	5420.0
75.00	16181.0
76.00	1371.0
77.00	264.0
77.70	130.0
78.90	1094.0
79.80	265.0
80.90	956.0
81.80	243.0
86.90	1802.0
87.90	1369.0
90.70	140.0
92.00	916.0
93.00	1614.0
94.00	3826.0
95.00	33880.0
96.00	2215.0
104.00	142.0
104.80	112.0
106.00	125.0
116.80	332.0
119.10	140.0
127.80	100.0
140.80	299.0
142.80	520.0
144.90	238.0
154.70	131.0
170.90	146.0
171.80	521.0
172.80	328.0
173.90	28688.0
174.90	2114.0
175.90	27544.0
176.90	2047.0
207.00	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.00	425.0
37.00	1669.0
38.00	1329.0
39.00	602.0
39.90	517.0
42.90	104.0
43.90	1299.0
45.00	408.0
45.80	262.0
47.00	488.0
47.90	171.0
48.90	1192.0
50.00	5350.0
51.00	1843.0
55.00	134.0
56.00	486.0
57.00	954.0
60.00	310.0
61.00	1582.0
62.00	1429.0
63.00	1376.0
63.90	194.0
65.00	337.0
67.10	152.0
67.90	2961.0
69.00	3161.0
70.00	275.0
71.90	170.0
73.00	1537.0
74.00	5504.0
75.00	16181.0
76.00	1286.0
77.00	294.0
78.90	1065.0
79.80	305.0
80.90	936.0
81.80	321.0
87.00	1826.0
87.80	1306.0
90.70	168.0
92.00	1050.0
93.00	1617.0
94.00	3821.0
95.00	33960.0
96.00	2257.0
103.90	133.0
106.00	119.0
116.10	101.0
116.90	247.0
118.00	108.0
119.00	176.0
127.80	109.0
140.80	304.0
142.80	519.0
144.90	233.0
154.70	181.0
170.90	154.0
171.80	509.0
172.90	366.0
173.90	29528.0
174.90	2159.0
175.90	28416.0
176.90	2104.0
207.00	209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	435.0
37.00	1411.0
38.00	1277.0
39.00	560.0
39.90	477.0
43.00	145.0
43.90	1324.0
45.00	436.0
45.90	281.0
47.00	470.0
47.90	174.0
48.90	1078.0
50.00	4904.0
51.00	1710.0
56.00	420.0
57.00	780.0
60.00	254.0
61.00	1587.0
62.00	1281.0
63.10	1229.0
63.90	153.0
65.00	387.0
67.10	122.0
68.00	2706.0
69.00	3031.0
70.00	245.0
72.00	129.0
73.00	1406.0
74.00	5129.0
75.00	14946.0
76.00	1130.0
77.00	266.0
77.80	160.0
78.90	917.0
79.80	304.0
80.90	905.0
81.80	341.0
86.90	1632.0
87.80	1313.0
90.80	187.0
91.90	1126.0
93.00	1369.0
94.00	3505.0
95.00	31168.0
96.00	2047.0
103.90	125.0
106.10	127.0
111.90	117.0
116.90	174.0
118.00	103.0
119.00	191.0
127.80	113.0
140.80	267.0
142.80	390.0
144.90	203.0
154.70	203.0
170.90	142.0
171.80	509.0
172.90	389.0
173.90	27960.0
174.90	2045.0
175.90	26696.0
176.90	1750.0
207.00	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64