


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082422\
Data File : VV027488.D
Acq On : 24 Aug 2022 10:03
Operator : SY/MD
Sample : BFB359
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB359

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Aug 26 01:50:00 2022

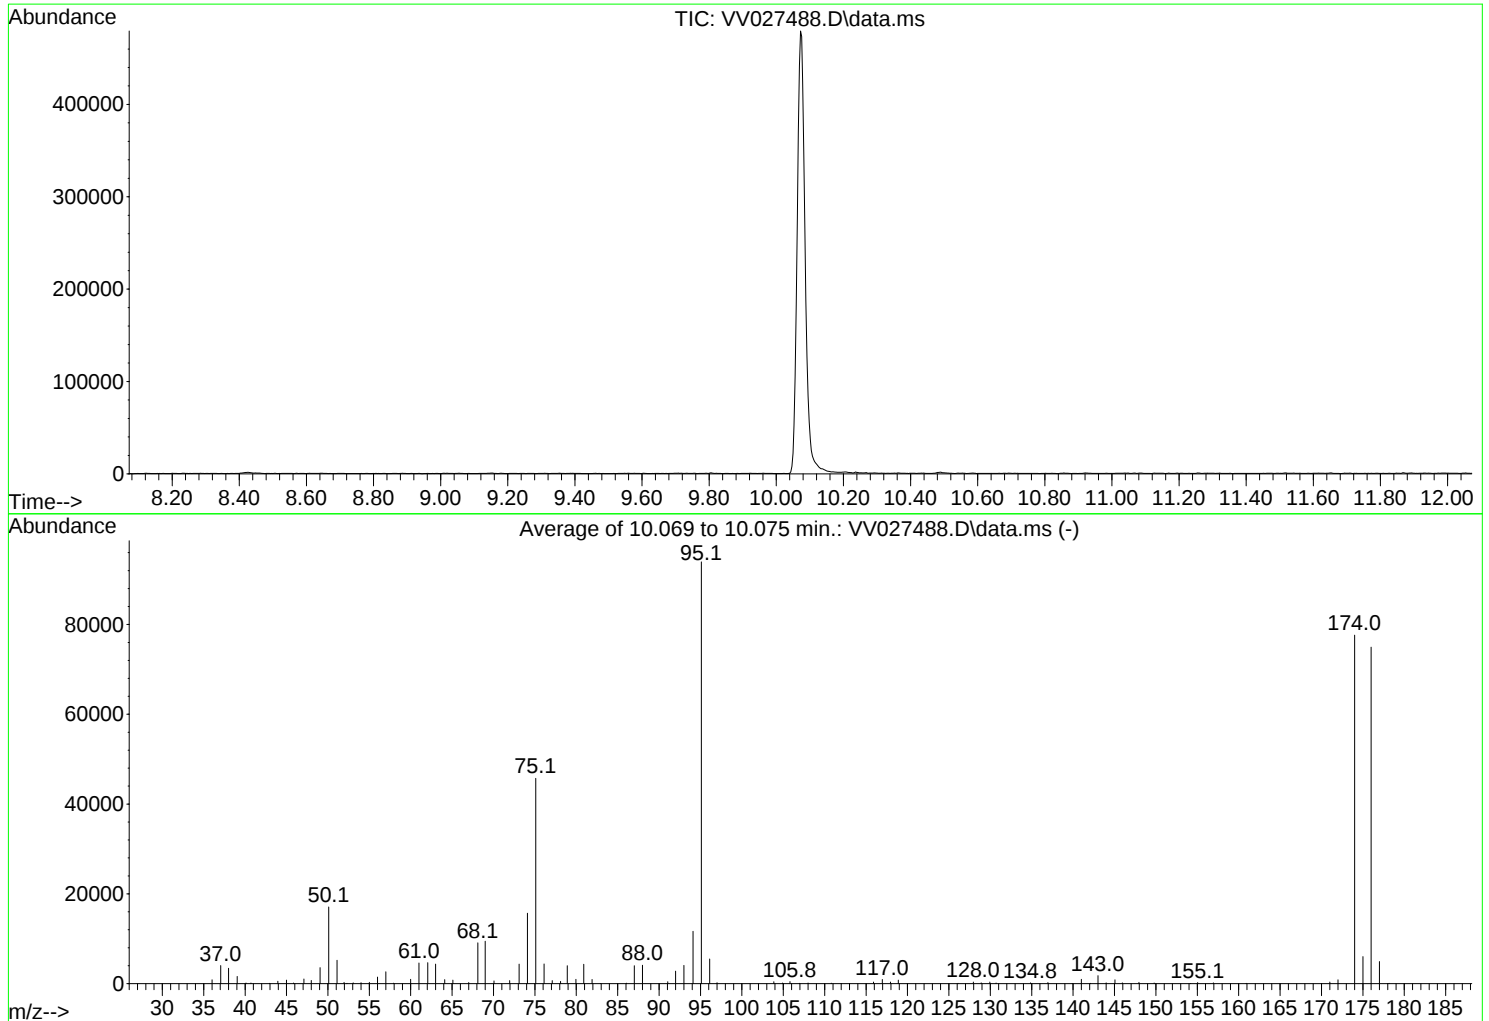

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	17057	PASS
75	95	30	80	48.7	45741	PASS
95	95	100	100	100.0	93952	PASS
96	95	5	9	5.8	5488	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.6	77624	PASS
175	174	5	9	7.8	6038	PASS
176	174	95	105	96.5	74941	PASS
177	176	5	10	6.6	4914	PASS

m/z	Abundance
40.10	132.0
43.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	846.0
37.10	4104.0
38.00	3337.0
39.00	1524.0
40.10	247.0
40.70	134.0
44.00	703.0
45.00	744.0
45.80	168.0
47.10	1050.0
48.00	710.0
49.10	3419.0
50.10	16306.0
51.10	5069.0
51.90	240.0
52.30	233.0
53.10	184.0
54.00	188.0
55.00	268.0
56.00	1444.0
57.00	2629.0
58.00	121.0
60.00	1010.0
61.00	4198.0
62.00	4445.0
63.00	4389.0
64.00	819.0
65.10	688.0
67.00	201.0
68.10	8674.0
69.00	9151.0
70.10	622.0
71.90	639.0
73.10	4273.0
74.10	15236.0
75.10	43544.0
76.10	4414.0
77.10	675.0
78.10	474.0
78.90	3771.0
79.90	955.0
80.90	3896.0
81.90	849.0
86.00	158.0
87.00	3861.0
88.00	3975.0
91.10	410.0
92.00	2601.0
93.00	3936.0
94.10	11044.0
95.10	88376.0
96.10	5131.0
97.00	190.0
103.90	460.0
104.90	155.0
105.80	442.0
107.00	104.0
108.00	160.0
110.80	116.0
112.00	102.0
113.00	105.0
115.90	362.0
116.90	834.0
118.00	361.0
118.90	667.0
126.10	108.0
128.00	333.0
128.80	177.0
129.90	373.0
130.60	116.0
134.80	157.0
137.00	190.0
141.00	914.0
143.00	1664.0
144.00	150.0
145.00	902.0
145.90	185.0
148.00	297.0
149.80	110.0
155.10	239.0
157.00	181.0
160.90	115.0
171.00	325.0
172.00	874.0
174.00	73480.0
175.00	5986.0
176.00	70008.0
177.00	4867.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	865.0
37.10	4085.0
38.00	3512.0
39.10	1674.0
40.10	274.0
40.70	138.0
42.90	102.0
44.00	822.0
45.00	856.0
45.80	159.0
47.10	1062.0
48.00	741.0
49.00	3642.0
50.10	17600.0
51.10	5350.0
51.90	284.0
53.10	185.0
54.00	221.0
55.00	312.0
56.00	1552.0
57.00	2728.0
58.00	128.0
60.00	986.0
61.00	4730.0
62.10	4764.0
63.00	4497.0
64.10	881.0
65.10	774.0
67.00	248.0
68.10	9427.0
69.00	9713.0
70.10	624.0
71.90	688.0
73.10	4533.0
74.10	16086.0
75.10	47176.0
76.10	4544.0
77.10	695.0
78.10	532.0
78.90	4042.0
79.90	1009.0
80.90	4435.0
81.90	945.0
86.10	163.0
87.00	4193.0
88.00	4274.0
91.00	446.0
92.00	2830.0
93.00	4195.0
94.10	12069.0
95.10	97216.0
96.10	5594.0
97.00	233.0
103.80	453.0
104.90	157.0
105.80	479.0
106.90	100.0
108.00	157.0
110.80	130.0
115.90	397.0
117.00	935.0
118.00	368.0
118.90	821.0
126.10	120.0
128.00	375.0
128.90	208.0
129.90	360.0
130.70	156.0
134.90	172.0
136.90	247.0
141.00	1003.0
143.00	1843.0
144.00	184.0
145.00	868.0
145.90	195.0
148.00	301.0
149.80	152.0
154.20	108.0
155.10	244.0
156.90	188.0
160.90	110.0
171.00	383.0
172.00	899.0
174.00	79952.0
175.00	6231.0
176.00	77152.0
177.00	5083.0
178.20	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	851.0
37.00	3875.0
38.00	3399.0
39.10	1650.0
40.10	260.0
40.70	123.0
43.00	127.0
44.00	853.0
45.00	783.0
45.90	130.0
47.10	956.0
48.00	720.0
49.00	3689.0
50.10	17264.0
51.10	5148.0
52.00	327.0
52.90	167.0
54.00	244.0
55.00	329.0
56.00	1446.0
57.00	2566.0
57.90	110.0
60.00	880.0
61.00	4846.0
62.10	4802.0
63.00	4179.0
64.20	932.0
65.10	851.0
67.00	280.0
68.10	9143.0
69.00	9462.0
70.00	575.0
72.00	672.0
73.10	4294.0
74.10	15716.0
75.10	46504.0
76.10	4175.0
77.10	630.0
78.10	525.0
78.90	4124.0
80.00	954.0
80.90	4588.0
81.90	958.0
82.90	125.0
87.00	3922.0
88.00	4024.0
91.00	431.0
92.00	2908.0
93.00	4091.0
94.10	11837.0
95.10	96264.0
96.10	5739.0
97.00	239.0
103.90	418.0
104.90	161.0
105.80	473.0
108.00	117.0
110.80	129.0
115.90	365.0
117.00	972.0
117.90	363.0
118.90	920.0
127.90	354.0
129.00	212.0
130.00	329.0
130.80	157.0
134.90	194.0
136.90	277.0
139.90	107.0
141.00	992.0
142.10	225.0
143.00	1860.0
144.00	171.0
145.10	789.0
146.00	177.0
147.90	270.0
149.80	158.0
154.90	230.0
156.90	160.0
171.00	373.0
172.00	836.0
174.00	79440.0
175.00	5898.0
176.00	77664.0
177.00	4791.0
178.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359