




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031911.D
 Acq On : 24 Aug 2023 15:59
 Operator : SY/MD
 Sample : 04158-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ3

Manual IntegrationsAPPROVED

Quant Time: Aug 25 00:59:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 25 00:56:34 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/25/2023
 Supervised By :Semsettin Yesilyurt 08/25/2023

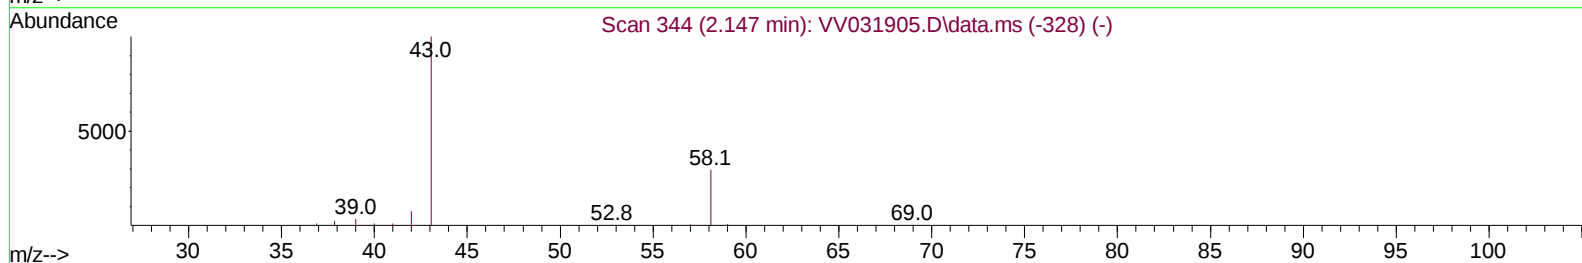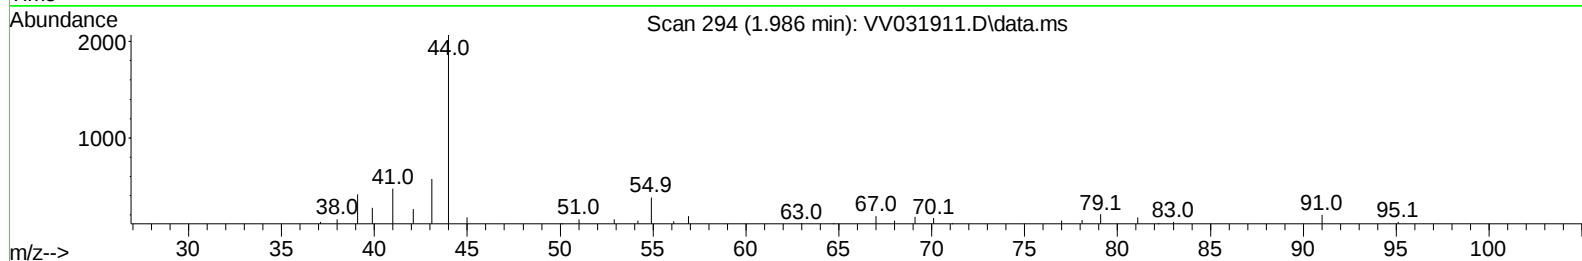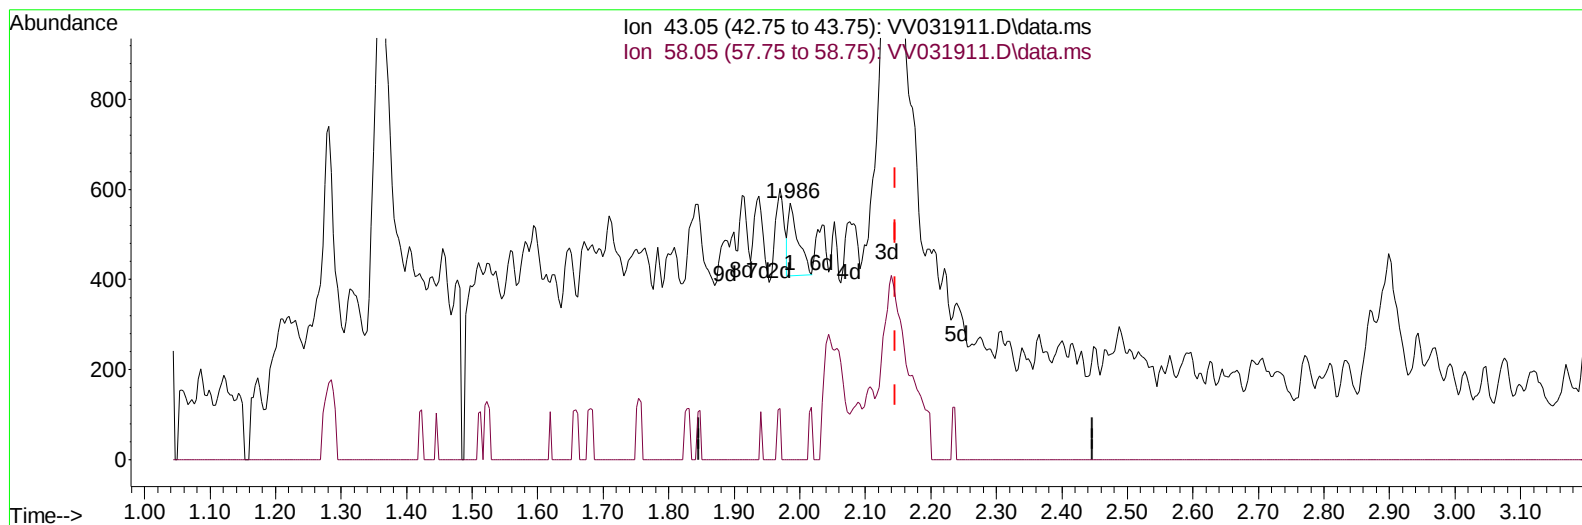

TIC: VV031911.D\data.ms

(13) Acetone (T)

1.986min (-0.161) 0.16 ug/L

response 170

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	25.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031911.D
 Acq On : 24 Aug 2023 15:59
 Operator : SY/MD
 Sample : 04158-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ3

Manual IntegrationsAPPROVED

Quant Time: Aug 25 00:59:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 25 00:56:34 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/25/2023
 Supervised By :Semsettin Yesilyurt 08/25/2023

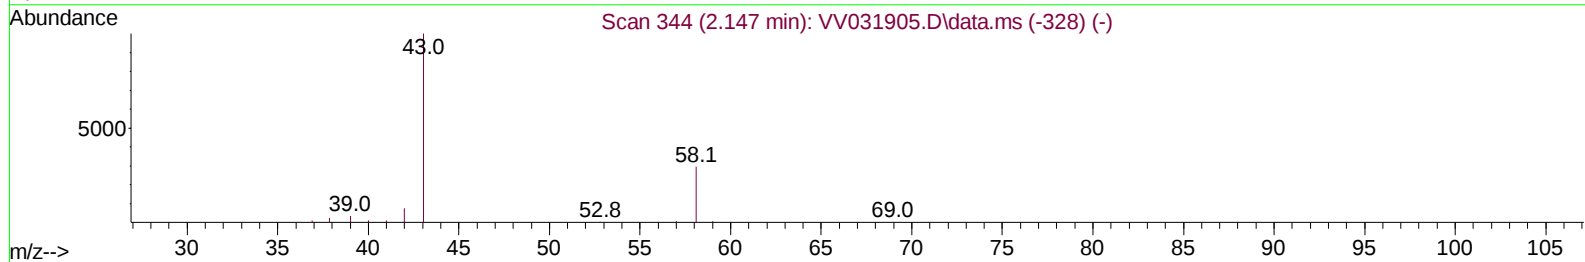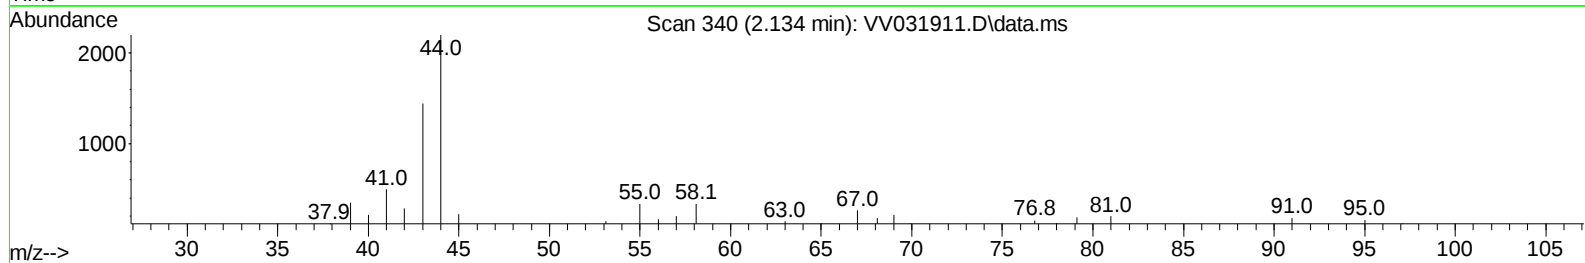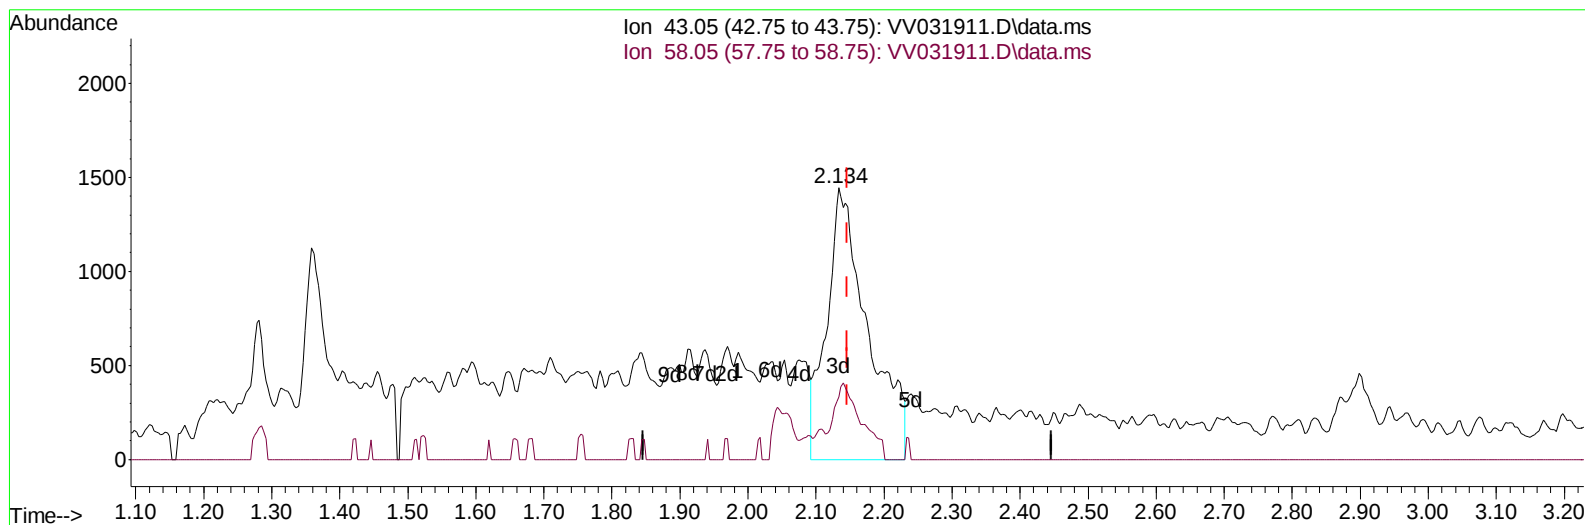

TIC: VV031911.D\data.ms

(13) Acetone (T)

2.134min (-0.013) 5.82 ug/L m

response 6088

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	0.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031911.D
 Acq On : 24 Aug 2023 15:59
 Operator : SY/MD
 Sample : 04158-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ3

Manual IntegrationsAPPROVED

Quant Time: Aug 25 00:59:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 25 00:56:34 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/25/2023
 Supervised By :Semsettin Yesilyurt 08/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	108611	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	101520	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	53531	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	0.000	65	0d	0.000	ug/L	
Spiked Amount 5.000	Range 40 - 130		Recovery =	0.000%#		
7) Chloroethane-d5	1.536	69	20780	4.945	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	98.800%		
11) 1,1-Dichloroethene-d2	2.063	65	8955	4.148	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	83.000%		
20) 2-Butanone-d5	3.815	46	112613	63.418	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	126.840%		
24) Chloroform-d	4.256	84	60442	4.868	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.400%		
26) 1,2-Dichloroethane-d4	4.950	65	32875	5.139	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	102.800%		
32) Benzene-d6	4.966	84	120159	5.201	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	104.000%		
36) 1,2-Dichloropropane-d6	5.995	67	42222	5.183	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	103.600%		
41) Toluene-d8	7.249	98	78001	3.639	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	72.800%		
43) trans-1,3-Dichloroprop...	7.564	79	11841	3.986	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	79.800%		
46) 2-Hexanone-d5	8.030	63	91111	57.528	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	115.060%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	32324	5.531	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	110.600%		
66) 1,2-Dichlorobenzene-d4	11.564	152	43994	5.075	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	101.400%		
Target Compounds						
13) Acetone	2.134	43	6088m	5.819	ug/L	
25) Chloroform	4.288	83	21196	1.822	ug/L	98
38) Bromodichloromethane	6.439	83	36555	4.384	ug/L	99
47) Tetrachloroethene	7.908	164	59934	13.727	ug/L	98
49) Dibromochloromethane	8.182	129	28608	5.953	ug/L	99
59) Bromoform	9.670	173	6915	2.734	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031911.D
Acq On : 24 Aug 2023 15:59
Operator : SY/MD
Sample : 04158-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/25/2023
Supervised By :Semsettin Yesilyurt 08/25/2023

Quant Time: Aug 25 00:59:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 25 00:56:34 2023
Response via : Initial Calibration

