

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031884.D
 Acq On : 23 Aug 2023 23:08
 Operator : SY/MD
 Sample : VV0824WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK355

Quant Time: Aug 24 04:52:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 24 04:46:53 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.538	114	112393	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.789	117	106029	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.191	152	55138	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	20688	5.450	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.000%	
7) Chloroethane-d5		1.529	69	24179	5.560	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.200%	
11) 1,1-Dichloroethene-d2		2.056	65	12015	5.378	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	107.600%	
20) 2-Butanone-d5		3.834	46	86612	47.134	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.260%	
24) Chloroform-d		4.256	84	65231	5.077	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4		4.950	65	35648	5.385	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.600%	
32) Benzene-d6		4.963	84	129248	5.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.200%	
36) 1,2-Dichloropropane-d6		5.995	67	44381	5.216	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.400%	
41) Toluene-d8		7.246	98	115989	5.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%	
43) trans-1,3-Dichloroprop...		7.564	79	15527	5.005	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.000%	
46) 2-Hexanone-d5		8.034	63	84393	51.020	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.040%	
56) 1,1,2,2-Tetrachloroeth...		10.159	84	31506	5.162	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.200%	
66) 1,2-Dichlorobenzene-d4		11.564	152	47188	5.285	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%	
Target Compounds							Qvalue
16) Methylene chloride		2.452	84	5013	0.609	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031884.D
Acq On : 23 Aug 2023 23:08
Operator : SY/MD
Sample : VV0824WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK355

Quant Time: Aug 24 04:52:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 24 04:46:53 2023
Response via : Initial Calibration

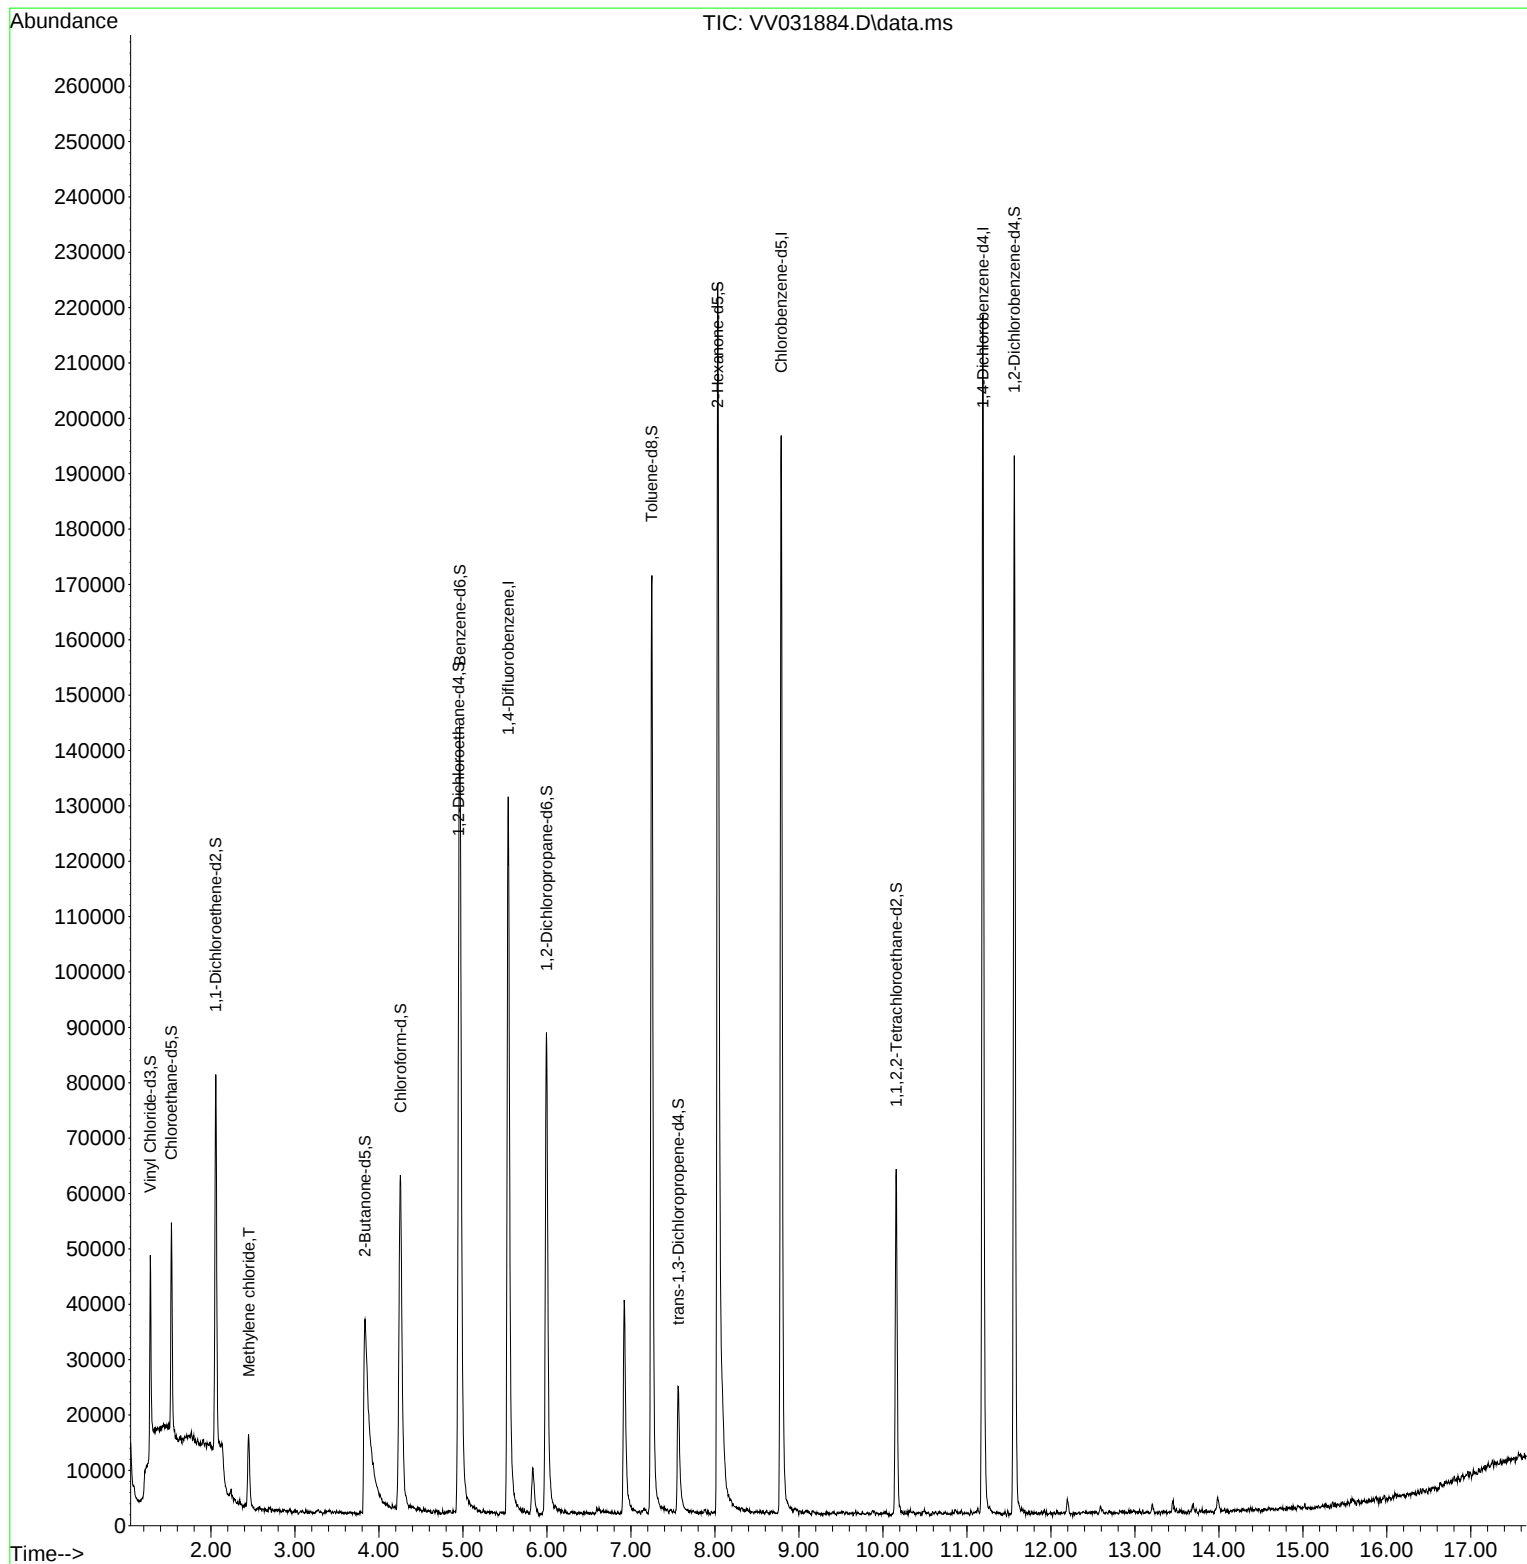

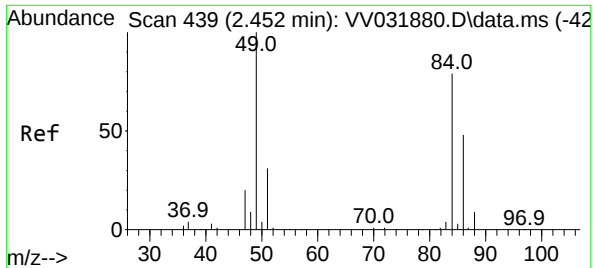

#16
Methylene chloride
Concen: 0.609 ug/L
RT: 2.452 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV031884.D
Acq: 23 Aug 2023 23:08

Instrument :
MSVOA_V
ClientSampleId :
VBLK355

Tgt Ion:	84	Resp:	5013
Ion	Ratio	Lower	Upper
84	100		
86	62.3	42.6	79.2
49	132.6	88.5	164.4

