

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031904.D
 Acq On : 24 Aug 2023 12:40
 Operator : SY/MD
 Sample : 04115-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Aug 25 00:52:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 24 04:46:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	117872	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	110262	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	57582	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	19084	4.794	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.800%
7) Chloroethane-d5	1.535	69	23039	5.052	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.000%
11) 1,1-Dichloroethene-d2	2.063	65	11789	5.032	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.600%
20) 2-Butanone-d5	3.818	46	98382	51.051	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.100%
24) Chloroform-d	4.252	84	65257	4.843	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	4.950	65	33567	4.835	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	4.963	84	127633	5.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	5.992	67	43376	4.902	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.000%
41) Toluene-d8	7.246	98	115903	4.978	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%
43) trans-1,3-Dichloroprop...	7.561	79	14849	4.602	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.000%
46) 2-Hexanone-d5	8.030	63	79027	45.942	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.880%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	29239	4.606	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	45368	4.865	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.452	84	2686	0.311	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031904.D
Acq On : 24 Aug 2023 12:40
Operator : SY/MD
Sample : 04115-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Aug 25 00:52:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 24 04:46:53 2023
Response via : Initial Calibration

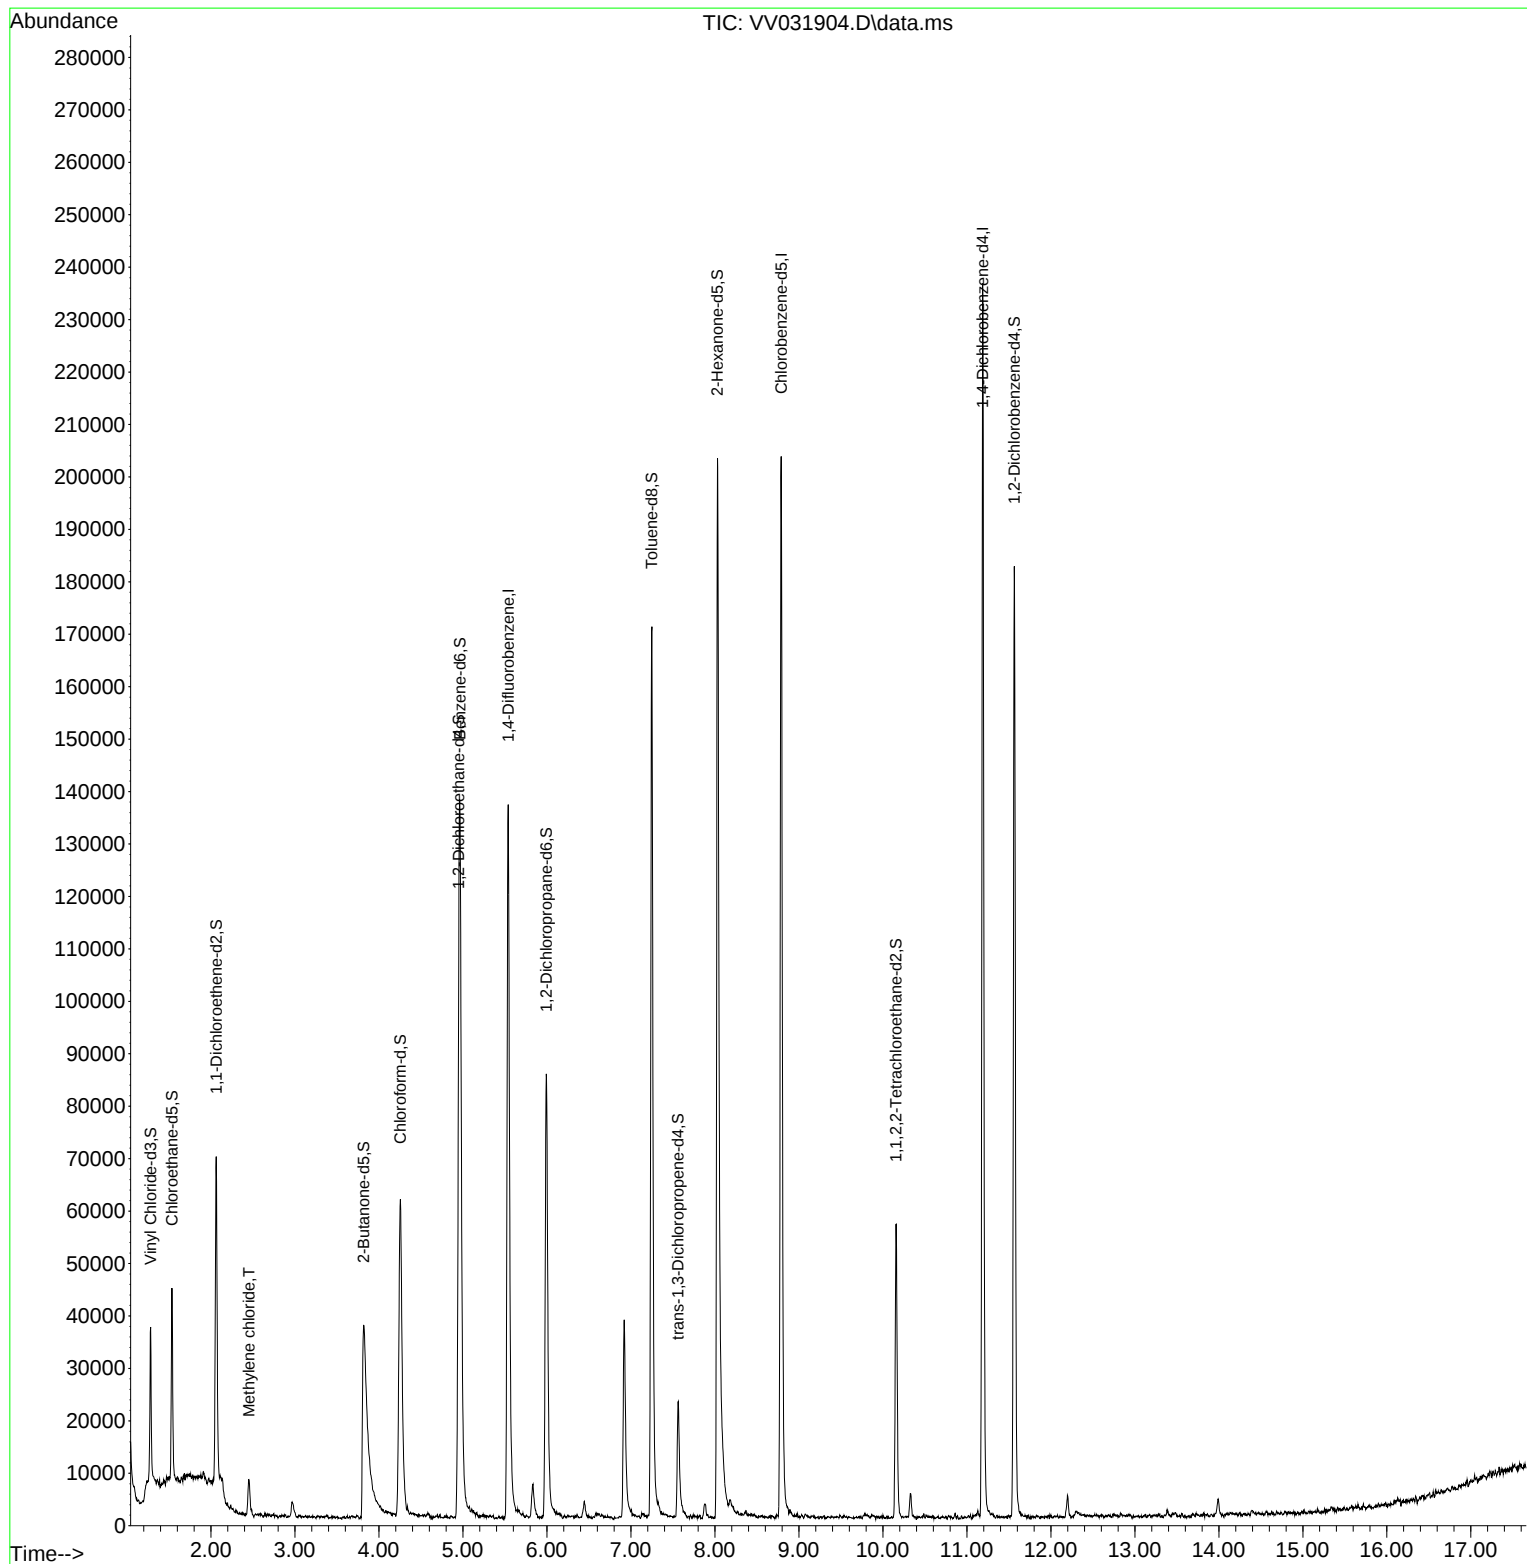

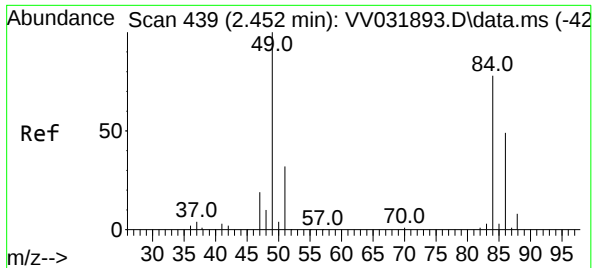

#16
Methylene chloride
Concen: 0.311 ug/L
RT: 2.452 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV031904.D
Acq: 24 Aug 2023 12:40

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84	Resp: 2686
Ion Ratio	Lower Upper
84 100	
86 60.7	42.6 79.2
49 112.8	88.5 164.4

