

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031896.D
 Acq On : 24 Aug 2023 09:26
 Operator : SY/MD
 Sample : 04115-05DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	33392	36989	7.96%	0.959%
2	1.536	147	154	166	rVB	39070	45264	9.74%	1.174%
3	2.063	309	318	331	rVB	69014	99542	21.41%	2.582%
4	3.822	849	865	919	rBV2	39770	196572	42.29%	5.098%
5	4.256	983	1000	1026	rBV	63310	168929	36.34%	4.381%
6	4.963	1204	1220	1252	rBV3	150485	392466	84.43%	10.179%
7	5.539	1385	1399	1426	rBV	141994	300670	64.68%	7.798%
8	5.831	1480	1490	1503	rBV7	4919	10826	2.33%	0.281%
9	5.995	1525	1541	1564	rBV	91836	200567	43.15%	5.202%
10	6.921	1818	1829	1849	rBV	40791	81431	17.52%	2.112%
11	7.246	1918	1930	1951	rBV	183172	331545	71.32%	8.599%
12	7.561	2019	2028	2048	rBV2	23841	48363	10.40%	1.254%
13	7.908	2117	2136	2155	rBV	169471	296265	63.73%	7.684%
14	8.034	2165	2175	2215	rBV	206670	464858	100.00%	12.056%
15	8.789	2397	2410	2436	rBV	209677	356560	76.70%	9.247%
16	10.159	2822	2836	2849	rBV	65518	107732	23.18%	2.794%
17	10.329	2878	2889	2898	rVB3	5526	9465	2.04%	0.245%
18	11.188	3146	3156	3179	rBV	243946	382753	82.34%	9.927%
19	11.564	3258	3273	3292	rBV	198018	320359	68.92%	8.308%
20	13.988	4017	4027	4037	rVB2	2683	4650	1.00%	0.121%




Sum of corrected areas: 3855806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031896.D
Acq On : 24 Aug 2023 09:26
Operator : SY/MD
Sample : 04115-05DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

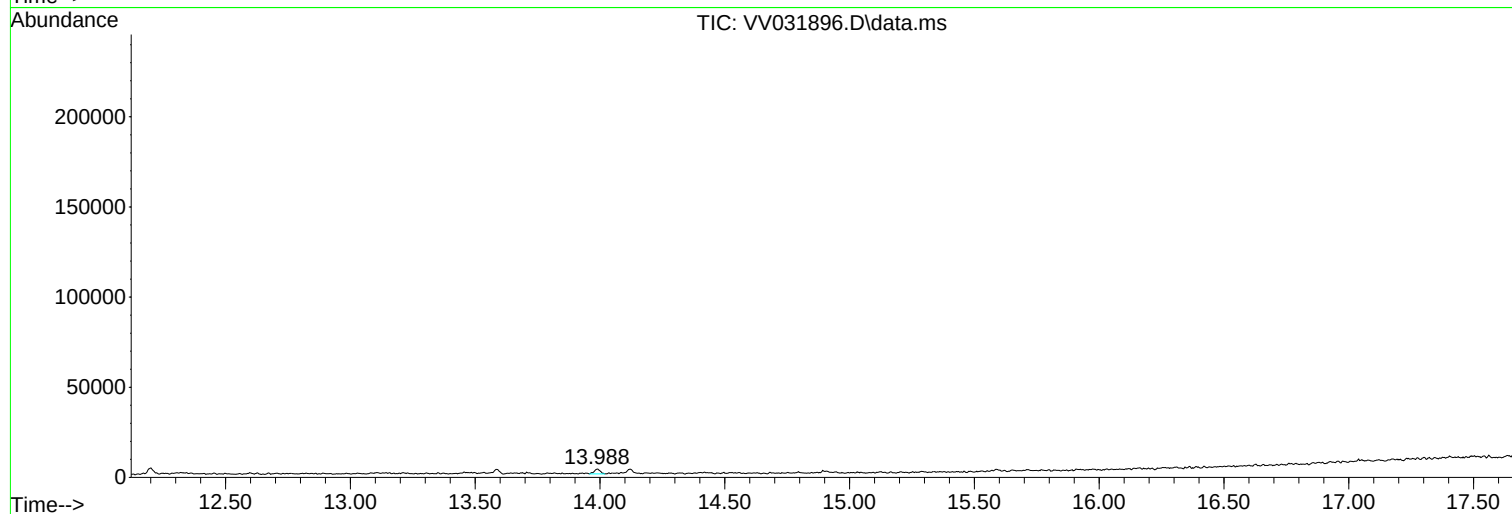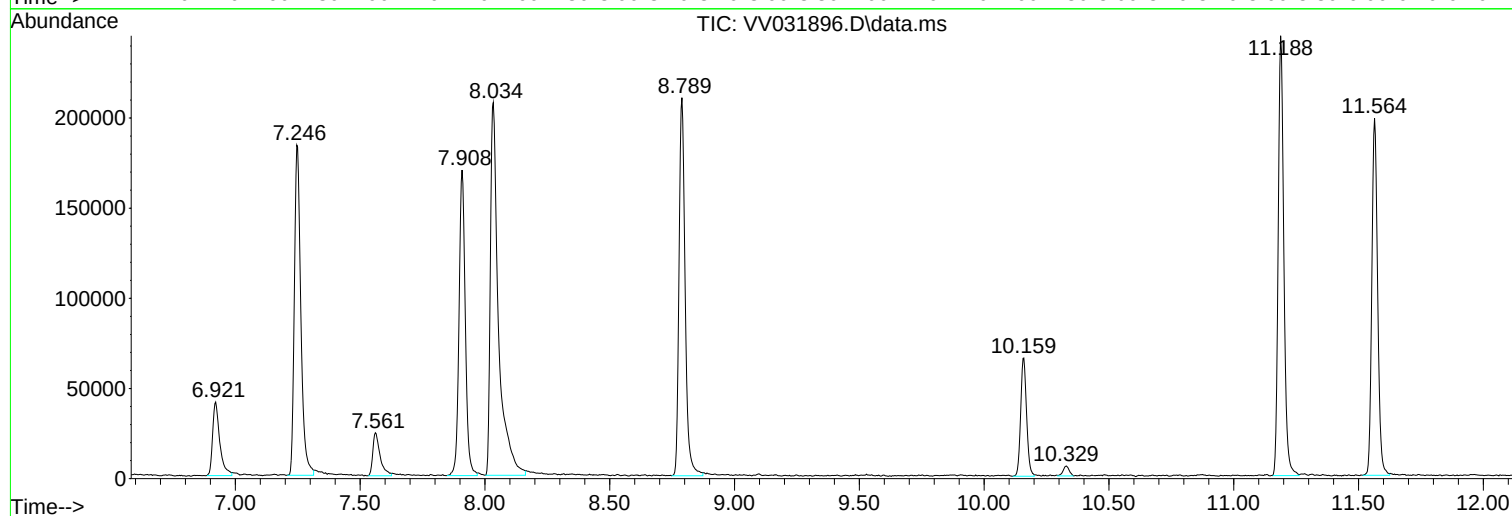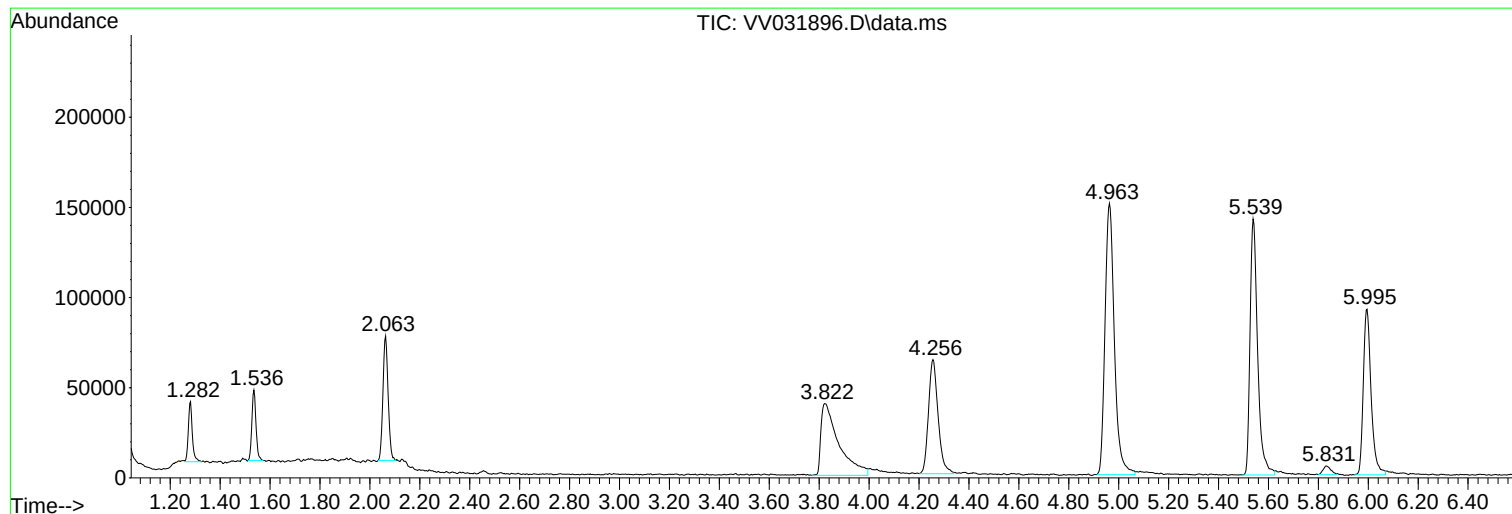

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031896.D
Acq On : 24 Aug 2023 09:26
Operator : SY/MD
Sample : 04115-05DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031896.D
Acq On : 24 Aug 2023 09:26
Operator : SY/MD
Sample : 04115-05DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc