

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031900.D
 Acq On : 24 Aug 2023 10:58
 Operator : SY/MD
 Sample : 04115-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	61	rBV	12190	14526	2.43%	0.340%
2	1.535	147	154	164	rBV	37077	43237	7.24%	1.011%
3	2.063	310	318	333	rVB	53760	78520	13.15%	1.836%
4	3.812	850	862	904	rBV3	55144	203377	34.07%	4.754%
5	4.259	986	1001	1031	rBV3	66044	207130	34.69%	4.842%
6	4.963	1204	1220	1246	rBV3	141124	366532	61.40%	8.568%
7	5.542	1388	1400	1425	rBV	146293	306568	51.35%	7.166%
8	5.834	1481	1491	1504	rBV6	6217	13488	2.26%	0.315%
9	5.995	1526	1541	1564	rBV	87390	189980	31.82%	4.441%
10	6.439	1668	1679	1699	rBV	49512	98219	16.45%	2.296%
11	6.921	1819	1829	1847	rBV	33045	66222	11.09%	1.548%
12	7.249	1919	1931	1956	rBV	129046	238768	39.99%	5.582%
13	7.564	2020	2029	2051	rBV2	18855	37425	6.27%	0.875%
14	7.908	2117	2136	2161	rBV	344242	597003	100.00%	13.956%
15	8.030	2165	2174	2210	rVV	210737	429036	71.86%	10.029%
16	8.181	2210	2221	2238	rVB	51582	97312	16.30%	2.275%
17	8.789	2399	2410	2437	rBV	217138	366605	61.41%	8.570%
18	9.673	2673	2685	2698	rBV3	14755	25691	4.30%	0.601%
19	9.767	2703	2714	2722	rBV7	4140	8103	1.36%	0.189%
20	10.159	2823	2836	2853	rBV	59424	96967	16.24%	2.267%
21	10.333	2877	2890	2901	rVB2	11030	19167	3.21%	0.448%
22	11.101	3121	3129	3141	rBV8	4753	8160	1.37%	0.191%
23	11.188	3146	3156	3176	rBV	247985	394029	66.00%	9.211%
24	11.490	3241	3250	3262	rBV	20052	32583	5.46%	0.762%
25	11.564	3262	3273	3282	rBV	187834	312086	52.28%	7.295%
26	12.197	3461	3470	3481	rVB2	5185	9241	1.55%	0.216%
27	12.297	3493	3501	3515	rBV9	5424	11294	1.89%	0.264%
28	13.988	4017	4027	4037	rBV	3995	6541	1.10%	0.153%




Sum of corrected areas: 4277810

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031900.D
Acq On : 24 Aug 2023 10:58
Operator : SY/MD
Sample : 04115-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

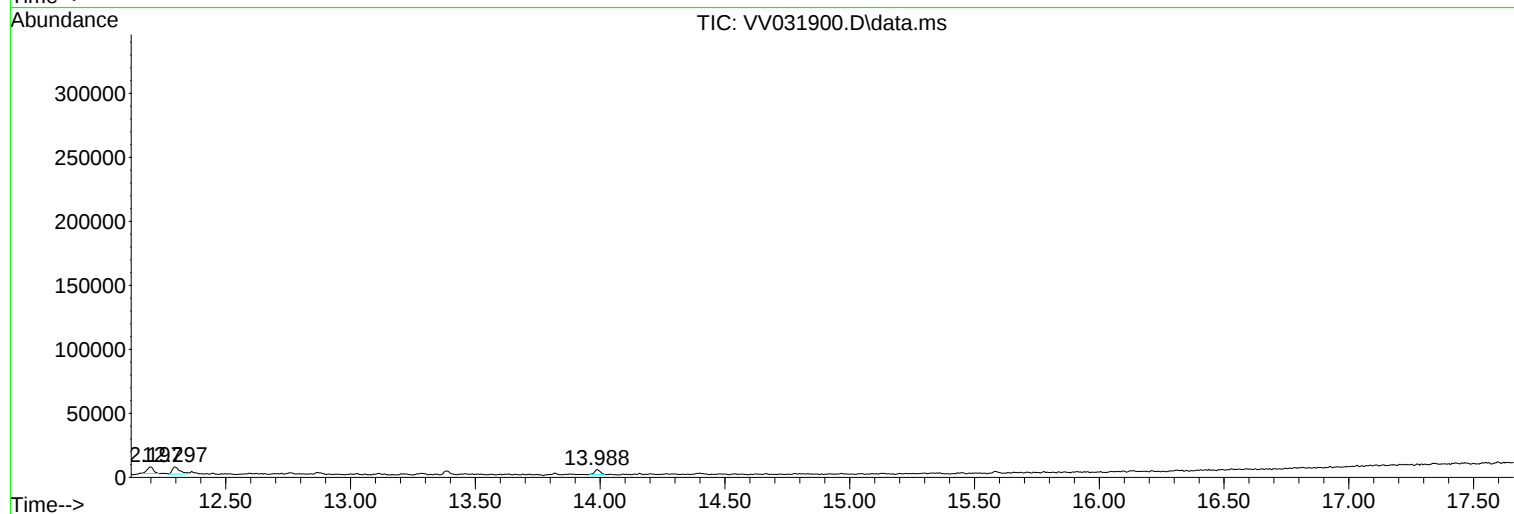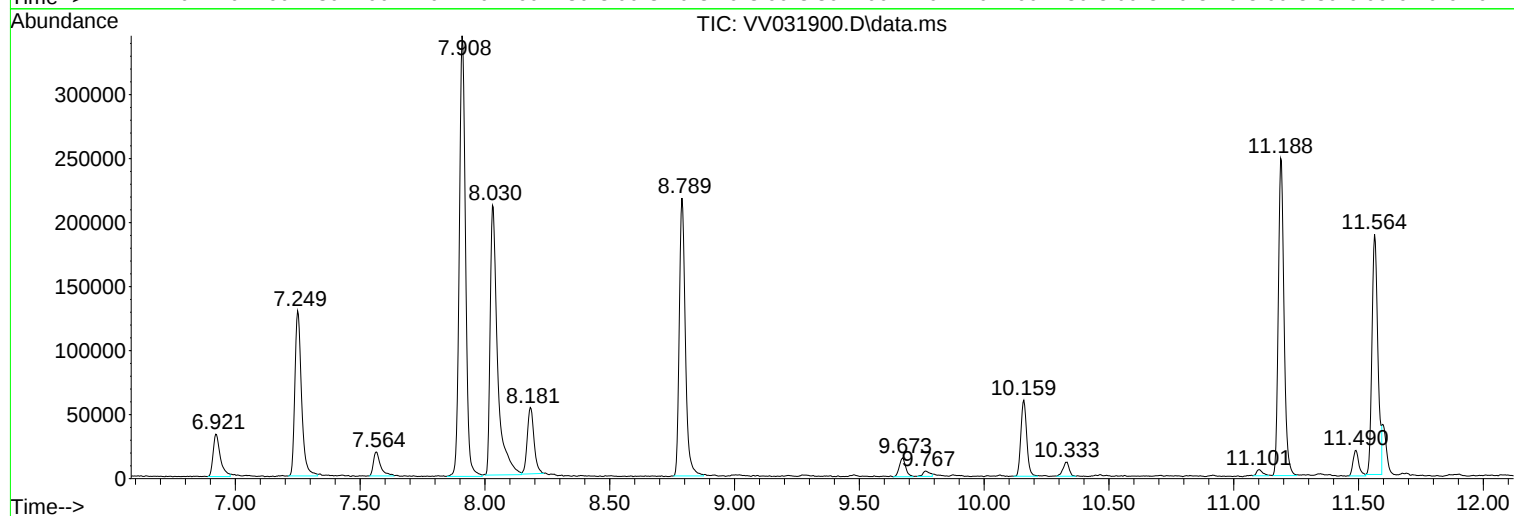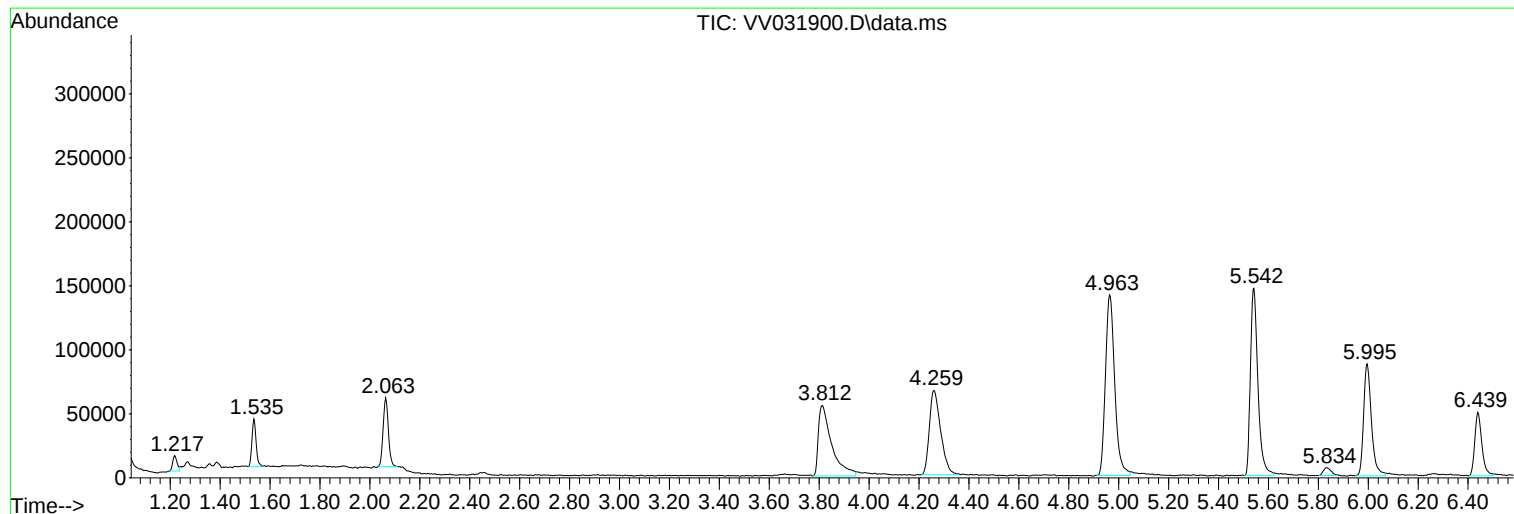

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031900.D
Acq On : 24 Aug 2023 10:58
Operator : SY/MD
Sample : 04115-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031900.D
Acq On : 24 Aug 2023 10:58
Operator : SY/MD
Sample : 04115-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc