

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031902.D
 Acq On : 24 Aug 2023 11:44
 Operator : SY/MD
 Sample : 04115-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.536	147	154	164	rBV	36523	41827	7.88%	1.017%
2	2.063	309	318	332	rBV	48877	74001	13.94%	1.799%
3	3.812	850	862	905	rBV2	54134	204465	38.52%	4.970%
4	4.259	985	1001	1033	rBV3	64913	205277	38.67%	4.990%
5	4.966	1204	1221	1250	rBV2	138048	359514	67.73%	8.739%
6	5.542	1386	1400	1424	rBV	129088	272892	51.41%	6.634%
7	5.834	1481	1491	1502	rBV6	5999	12530	2.36%	0.305%
8	5.995	1528	1541	1567	rBV	86097	185762	34.99%	4.516%
9	6.439	1667	1679	1700	rBV	47574	95956	18.08%	2.333%
10	6.924	1816	1830	1846	rBV	32337	65175	12.28%	1.584%
11	7.249	1918	1931	1962	rBV	126132	230284	43.38%	5.598%
12	7.564	2020	2029	2042	rBV	20366	38462	7.25%	0.935%
13	7.908	2117	2136	2162	rBV	306733	530839	100.00%	12.904%
14	8.030	2165	2174	2211	rVV	233593	474811	89.45%	11.542%
15	8.182	2211	2221	2241	rVB2	55738	104404	19.67%	2.538%
16	8.789	2396	2410	2432	rBV	196864	333495	62.82%	8.107%
17	9.673	2675	2685	2700	rBV	15038	26340	4.96%	0.640%
18	10.159	2825	2836	2850	rBV	62815	101749	19.17%	2.473%
19	10.329	2875	2889	2902	rVB5	13029	26326	4.96%	0.640%
20	11.107	3119	3131	3144	rBV7	3410	6286	1.18%	0.153%
21	11.188	3145	3156	3178	rVV	224576	357140	67.28%	8.682%
22	11.487	3241	3249	3259	rBV2	18188	29983	5.65%	0.729%
23	11.564	3262	3273	3282	rBV	185646	307999	58.02%	7.487%
24	12.197	3455	3470	3478	rBV	6367	12385	2.33%	0.301%
25	12.300	3492	3502	3513	rBV7	4332	8618	1.62%	0.209%
26	13.992	4019	4028	4035	rVB2	4383	7193	1.36%	0.175%




Sum of corrected areas: 4113713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031902.D
Acq On : 24 Aug 2023 11:44
Operator : SY/MD
Sample : 04115-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

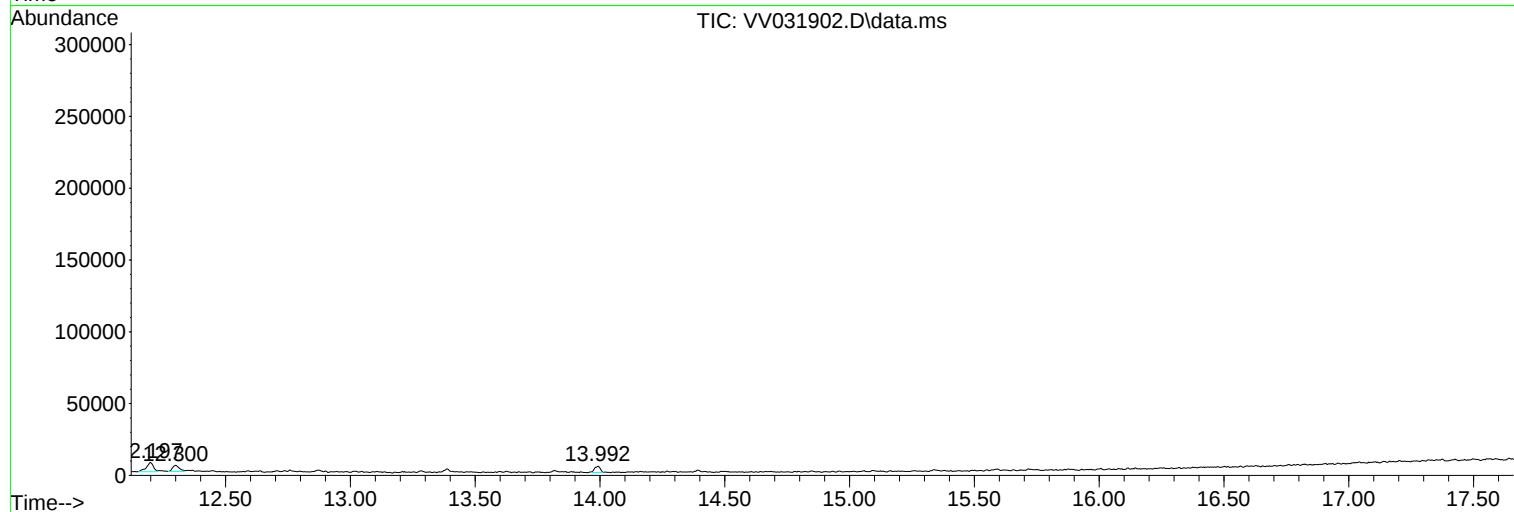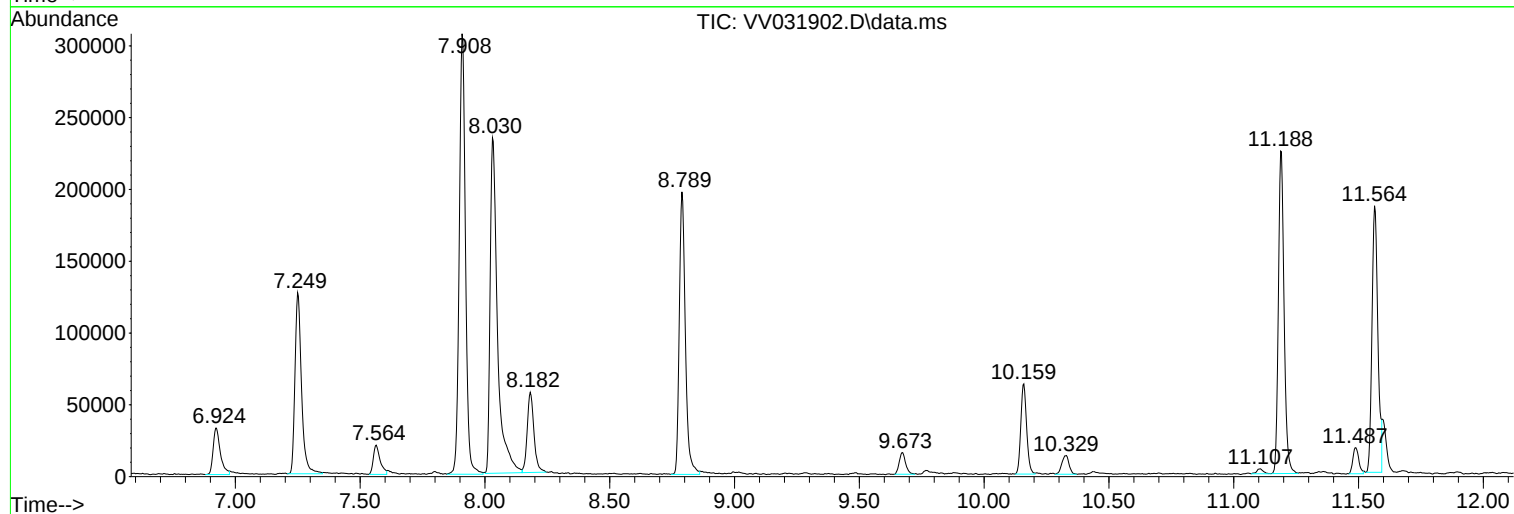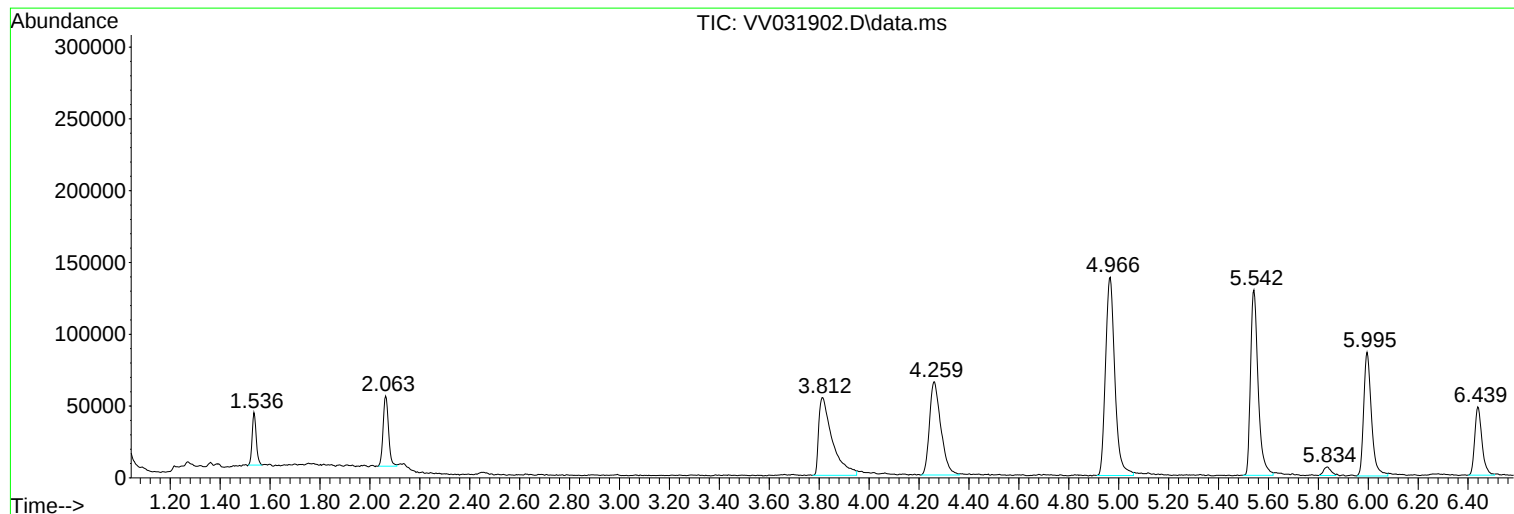

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031902.D
Acq On : 24 Aug 2023 11:44
Operator : SY/MD
Sample : 04115-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031902.D
Acq On : 24 Aug 2023 11:44
Operator : SY/MD
Sample : 04115-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc