

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031906.D
 Acq On : 24 Aug 2023 14:02
 Operator : SY/MD
 Sample : VV0824WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK357

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rVB	31504	33781	7.68%	0.996%
2	1.535	148	154	163	rVB	36257	40852	9.29%	1.204%
3	2.063	309	318	334	rVB	66652	97013	22.06%	2.859%
4	2.452	429	439	452	rVB2	5886	10406	2.37%	0.307%
5	2.973	589	601	615	rBV7	4166	8953	2.04%	0.264%
6	3.815	850	863	890	rBV2	33801	122406	27.83%	3.608%
7	4.252	983	999	1026	rVB	59492	157450	35.80%	4.641%
8	4.960	1201	1219	1251	rBV2	143252	375351	85.34%	11.063%
9	5.538	1387	1399	1430	rBV	141000	303280	68.95%	8.939%
10	5.831	1480	1490	1503	rBV2	6890	14570	3.31%	0.429%
11	5.992	1526	1540	1568	rBV	87484	188530	42.86%	5.557%
12	6.918	1817	1828	1844	rBV2	38058	76484	17.39%	2.254%
13	7.246	1918	1930	1950	rBV	173825	314049	71.40%	9.256%
14	7.561	2019	2028	2044	rBV	22466	43353	9.86%	1.278%
15	8.030	2164	2174	2218	rBV	191469	439851	100.00%	12.964%
16	8.789	2399	2410	2432	rBV	211083	361348	82.15%	10.650%
17	10.156	2825	2835	2852	rBV	56071	93132	21.17%	2.745%
18	11.188	3145	3156	3178	rBV	247448	392112	89.15%	11.557%
19	11.564	3262	3273	3296	rBV	185220	302938	68.87%	8.929%
20	13.448	3852	3859	3869	rBV	7732	12331	2.80%	0.363%
21	13.686	3925	3933	3942	rVB6	2947	4642	1.06%	0.137%




Sum of corrected areas: 3392832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031906.D
Acq On : 24 Aug 2023 14:02
Operator : SY/MD
Sample : VV0824WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

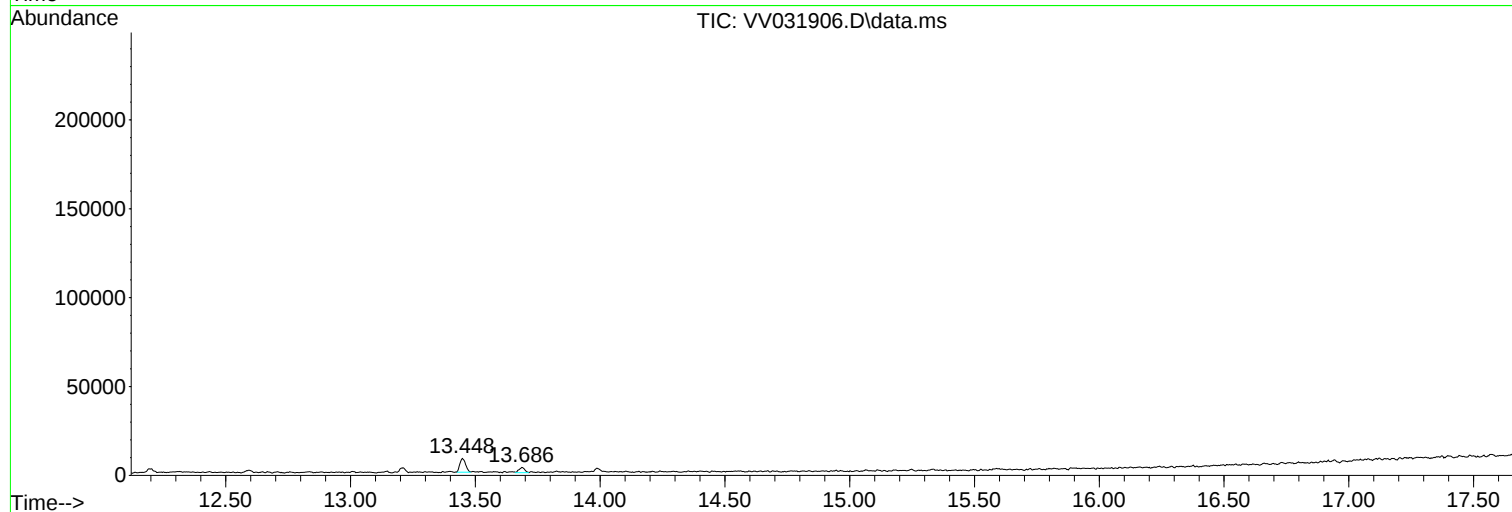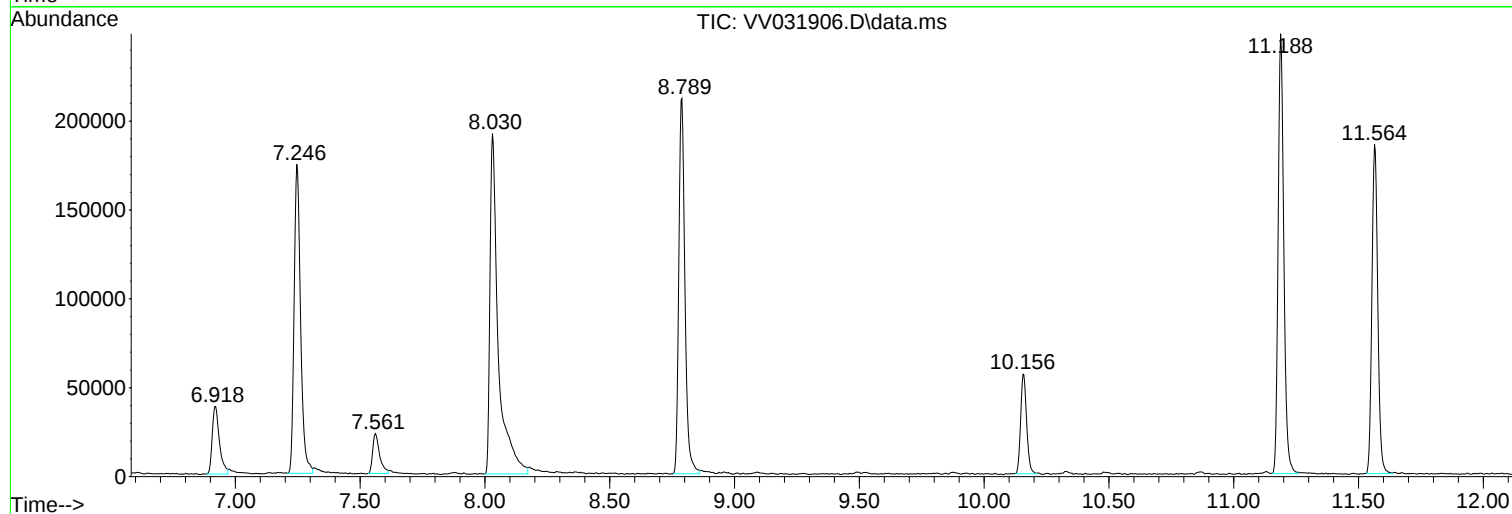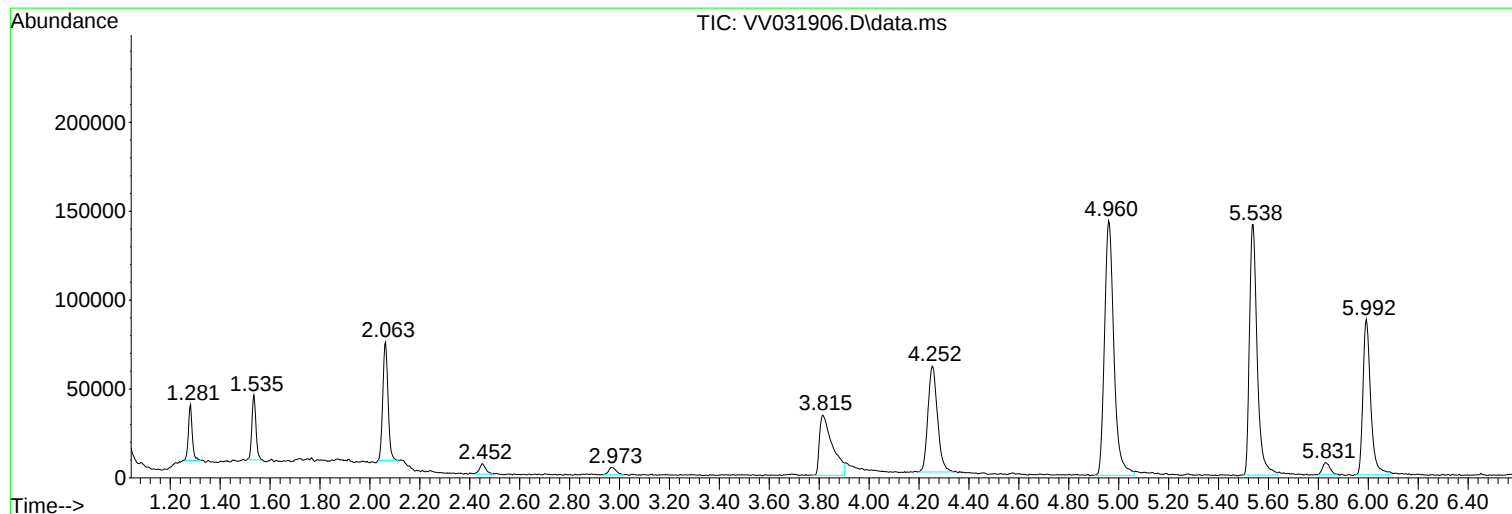

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031906.D
Acq On : 24 Aug 2023 14:02
Operator : SY/MD
Sample : VV0824WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031906.D
Acq On : 24 Aug 2023 14:02
Operator : SY/MD
Sample : VV0824WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc