

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031919.D
 Acq On : 24 Aug 2023 19:11
 Operator : SY/MD
 Sample : 04153-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH459

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	18	23	30	rVB2	6673	7482	1.55%	0.210%
2	1.281	68	75	85	rBV	25653	27684	5.72%	0.777%
3	1.535	148	154	164	rVB	31977	37398	7.72%	1.049%
4	2.063	309	318	335	rBV2	63400	102979	21.27%	2.889%
5	3.124	636	648	659	rVB2	4144	8682	1.79%	0.244%
6	3.818	853	864	901	rBV3	81882	272015	56.18%	7.631%
7	4.259	983	1001	1029	rBV4	62952	209390	43.25%	5.874%
8	4.963	1203	1220	1242	rBV2	129030	336168	69.43%	9.430%
9	5.538	1388	1399	1423	rBV	129606	273820	56.55%	7.681%
10	5.841	1481	1493	1514	rBV3	48077	104469	21.58%	2.931%
11	5.995	1528	1541	1561	rBV2	80843	172400	35.61%	4.836%
12	6.921	1818	1829	1848	rBV	34736	68214	14.09%	1.914%
13	7.249	1919	1931	1949	rBV	156335	278314	57.48%	7.807%
14	7.564	2018	2029	2048	rBV2	21250	42608	8.80%	1.195%
15	7.876	2117	2126	2133	rBV3	5906	11395	2.35%	0.320%
16	8.034	2162	2175	2216	rBV	229028	484186	100.00%	13.583%
17	8.789	2394	2410	2433	rBV	193090	331836	68.53%	9.309%
18	10.159	2824	2836	2851	rBV	64567	103046	21.28%	2.891%
19	10.329	2877	2889	2902	rBV3	14915	25492	5.26%	0.715%
20	11.191	3146	3157	3177	rBV	219654	350132	72.31%	9.822%
21	11.500	3244	3253	3263	rBV5	6999	14950	3.09%	0.419%
22	11.564	3263	3273	3302	rVB	174998	290712	60.04%	8.155%
23	12.201	3461	3471	3481	rVB2	7027	11344	2.34%	0.318%




Sum of corrected areas: 3564716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031919.D
Acq On : 24 Aug 2023 19:11
Operator : SY/MD
Sample : 04153-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH459

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

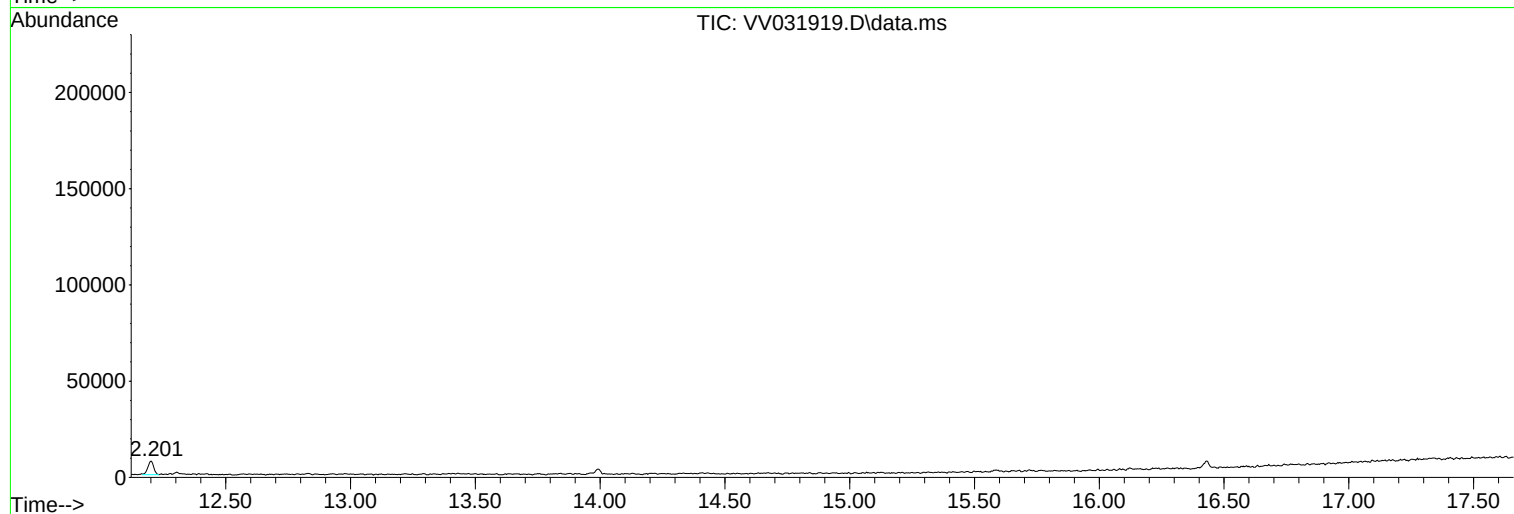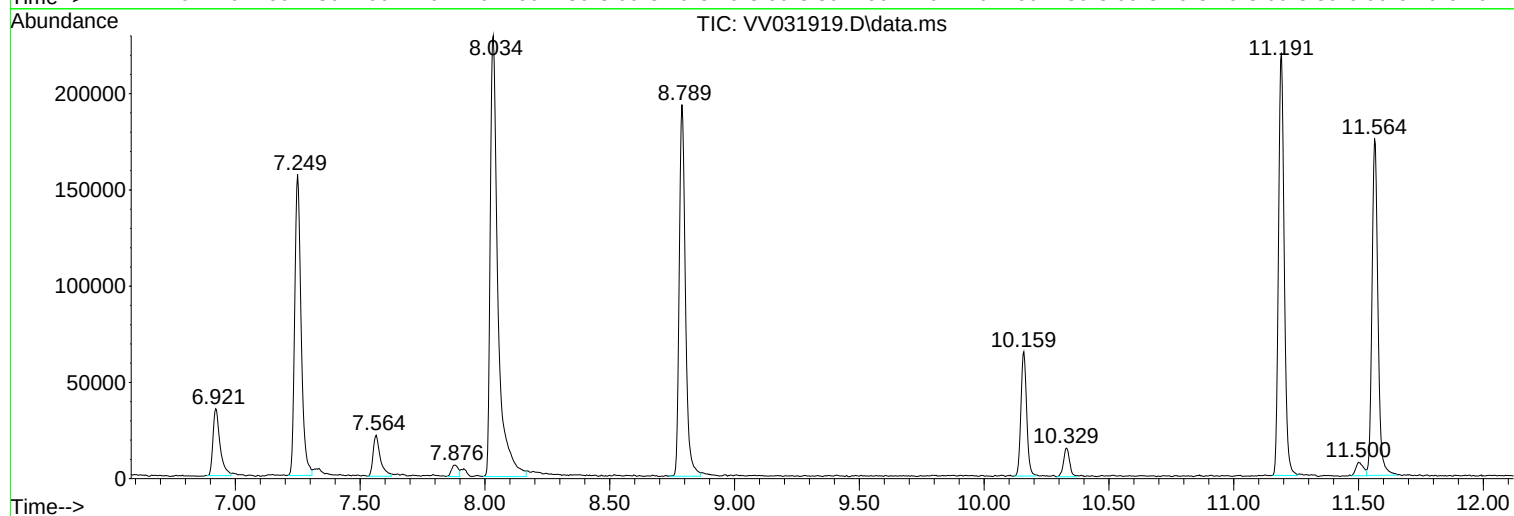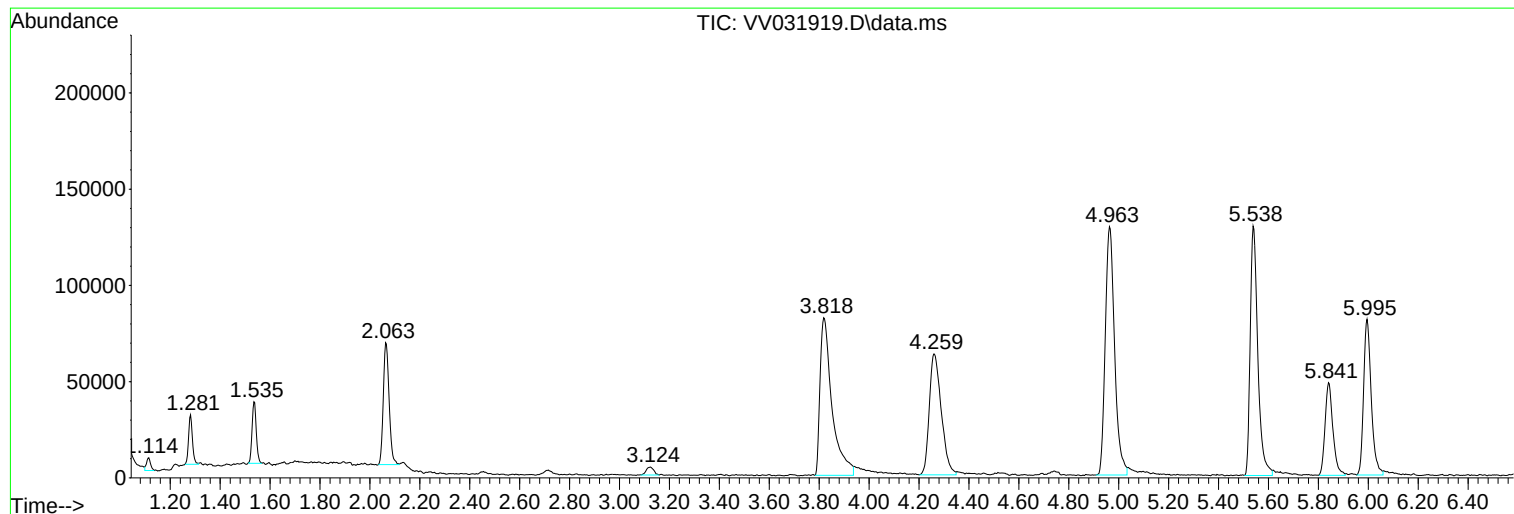

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031919.D
Acq On : 24 Aug 2023 19:11
Operator : SY/MD
Sample : 04153-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH459

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031919.D
Acq On : 24 Aug 2023 19:11
Operator : SY/MD
Sample : 04153-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH459

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc