

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
 Data File : VV031920.D
 Acq On : 24 Aug 2023 19:35
 Operator : SY/MD
 Sample : 04153-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH460

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	33	rVB2	17924	20422	2.09%	0.415%
2	1.281	69	75	83	rVB	27003	27323	2.80%	0.555%
3	1.535	148	154	169	rVB	34896	41852	4.29%	0.850%
4	2.069	309	320	340	rVB3	105631	188505	19.31%	3.829%
5	3.117	634	646	670	rBV2	17654	39765	4.07%	0.808%
6	3.818	849	864	907	rBV2	364437	976287	100.00%	19.830%
7	4.265	984	1003	1030	rBV4	80141	288680	29.57%	5.864%
8	4.741	1137	1151	1167	rVB5	5446	13009	1.33%	0.264%
9	4.963	1201	1220	1242	rBV2	135853	350762	35.93%	7.125%
10	5.538	1388	1399	1426	rBV	133256	285201	29.21%	5.793%
11	5.837	1480	1492	1520	rBV	224925	458459	46.96%	9.312%
12	5.995	1528	1541	1561	rBV	85660	177014	18.13%	3.595%
13	6.921	1819	1829	1850	rBV	36403	72495	7.43%	1.472%
14	7.249	1920	1931	1958	rBV	160308	295082	30.22%	5.994%
15	7.561	2019	2028	2048	rBV	21975	42780	4.38%	0.869%
16	8.030	2165	2174	2210	rBV	235839	491754	50.37%	9.988%
17	8.789	2399	2410	2436	rBV	202801	345404	35.38%	7.016%
18	10.159	2822	2836	2851	rBV	66009	107433	11.00%	2.182%
19	10.329	2880	2889	2901	rVB3	9251	14440	1.48%	0.293%
20	11.191	3146	3157	3173	rBV	228895	367334	37.63%	7.461%
21	11.496	3242	3252	3262	rBV2	13094	27513	2.82%	0.559%
22	11.564	3263	3273	3289	rVB	180411	291770	29.89%	5.926%




Sum of corrected areas: 4923284

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031920.D
Acq On : 24 Aug 2023 19:35
Operator : SY/MD
Sample : 04153-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH460

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

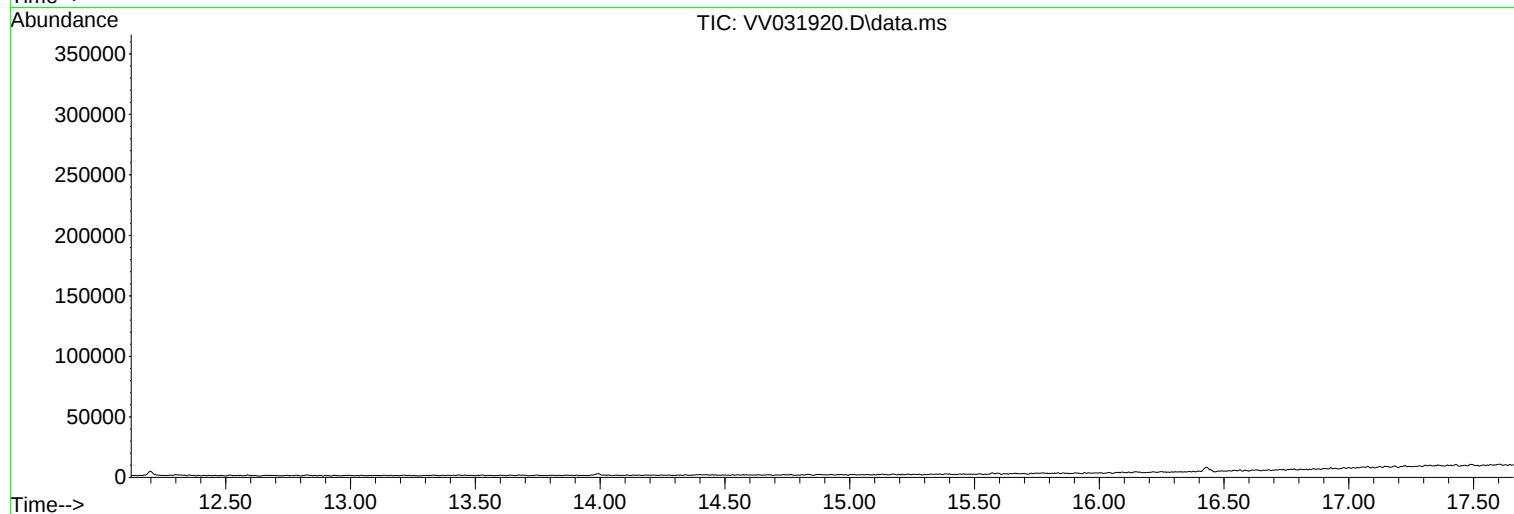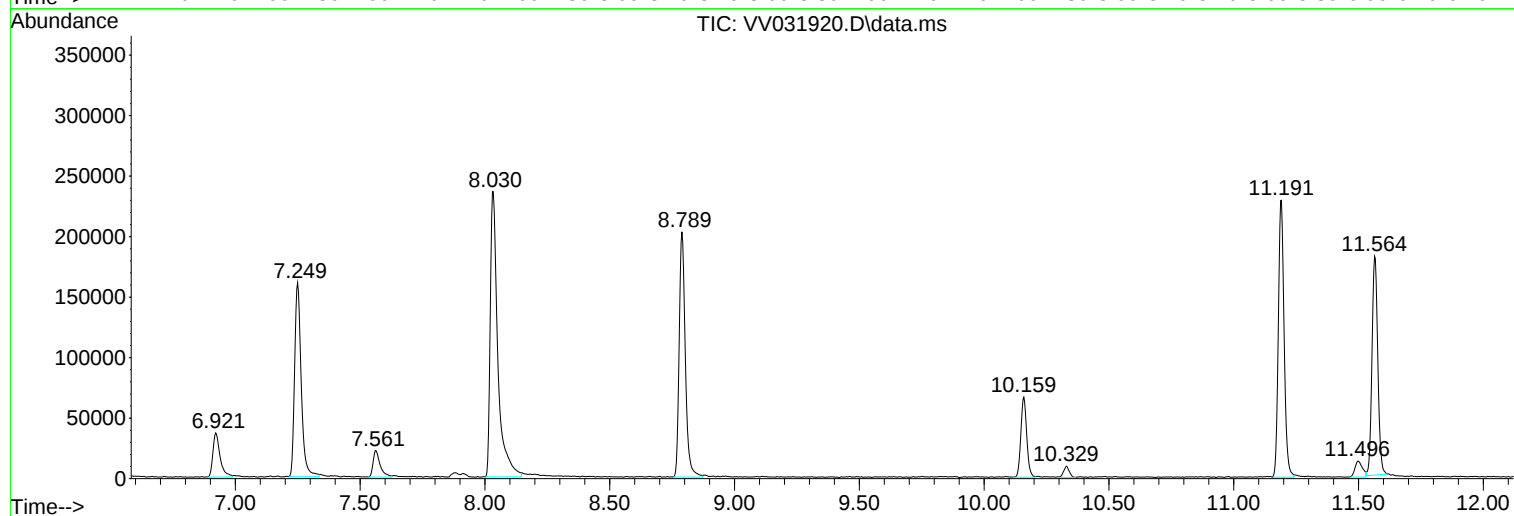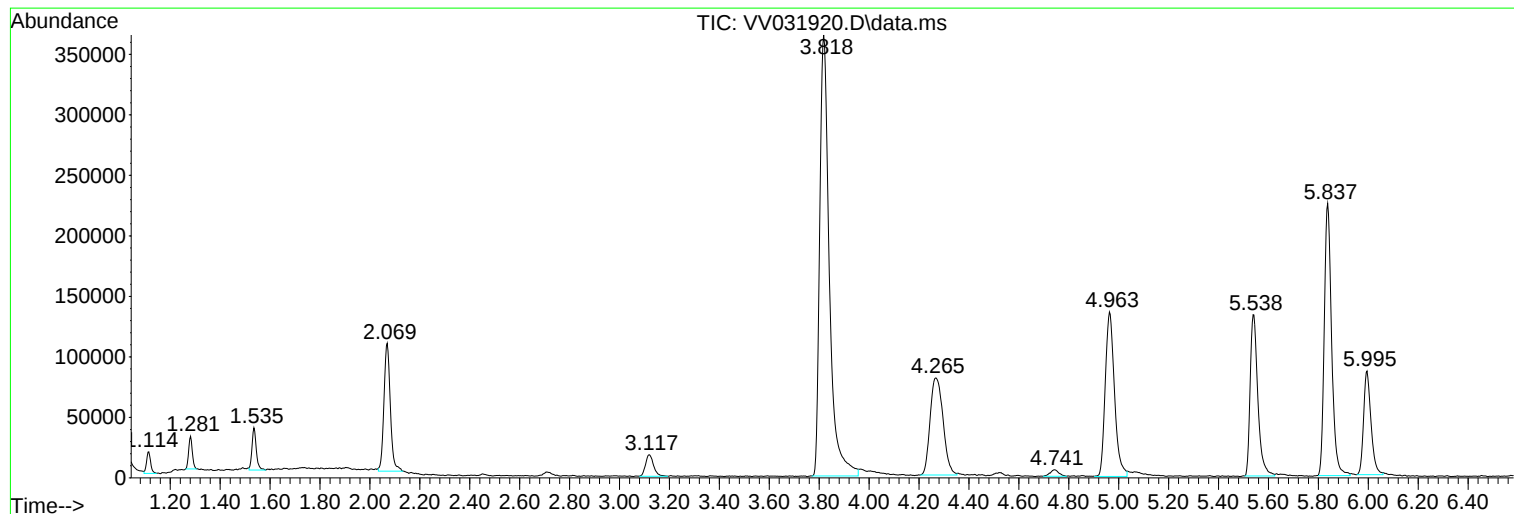

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031920.D
Acq On : 24 Aug 2023 19:35
Operator : SY/MD
Sample : 04153-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH460

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031920.D
Acq On : 24 Aug 2023 19:35
Operator : SY/MD
Sample : 04153-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH460

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------