
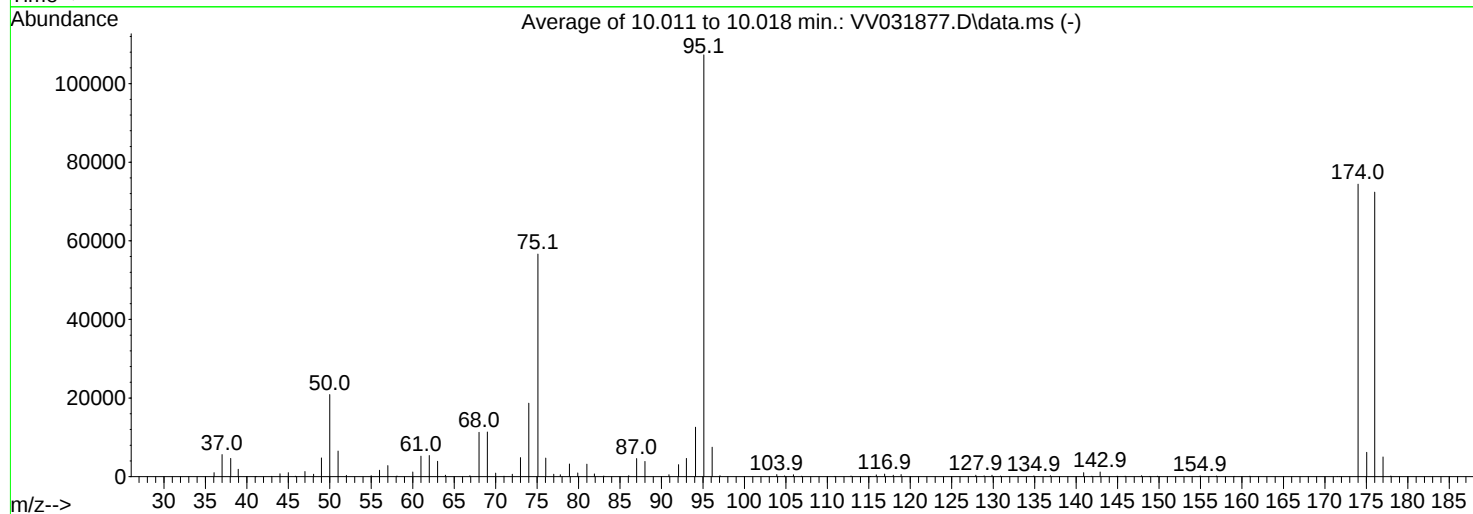


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082423\
Data File : VV031877.D
Acq On : 23 Aug 2023 18:18
Operator : SY/MD
Sample : BFB288
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB288

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Aug 25 00:56:34 2023

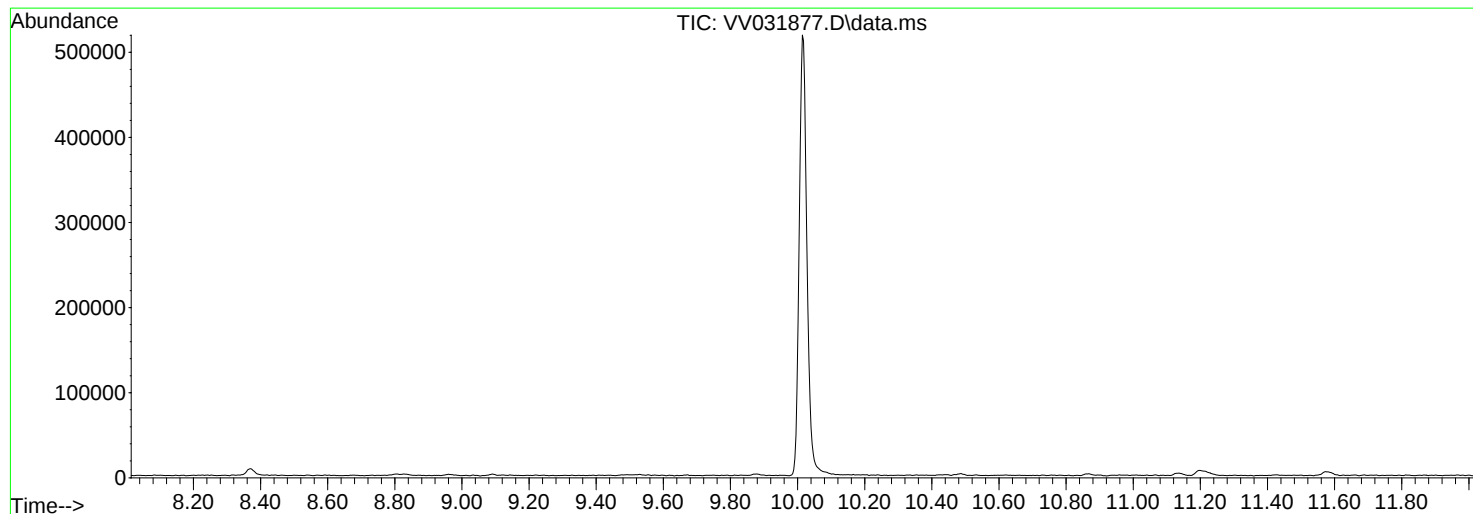

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	20872	PASS
75	95	30	80	52.7	56611	PASS
95	95	100	100	100.0	107320	PASS
96	95	5	9	7.0	7500	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.4	74432	PASS
175	174	5	9	8.3	6204	PASS
176	174	95	105	97.3	72389	PASS
177	176	5	10	6.9	5016	PASS

m/z	Abundance
38.90	195.0
40.00	252.0
41.00	247.0
42.00	205.0
43.00	227.0
44.00	756.0
55.10	222.0
56.00	113.0
57.00	127.0
66.90	129.0
69.00	124.0
77.00	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.10	1015.0
37.00	5524.0
38.00	4665.0
39.00	2021.0
40.00	293.0
41.00	273.0
42.10	151.0
43.00	278.0
44.00	1528.0
45.00	951.0
45.90	109.0
47.00	1358.0
48.10	548.0
49.00	4600.0
50.00	20200.0
51.00	6368.0
52.00	357.0
55.00	471.0
56.00	1740.0
57.00	2908.0
58.10	150.0
60.00	1073.0
61.00	5069.0
62.00	5059.0
63.00	3799.0
63.90	321.0
66.90	344.0
68.00	11088.0
69.00	11068.0
70.00	969.0
71.00	141.0
72.00	577.0
73.00	4532.0
74.00	17768.0
75.10	54216.0
76.00	4581.0
77.00	741.0
77.80	448.0
78.90	3142.0
79.90	896.0
81.00	3068.0
81.90	643.0
83.00	183.0
86.10	232.0
87.00	4497.0
88.00	3748.0
90.90	493.0
92.00	2883.0
93.00	4420.0
94.10	12141.0
95.10	102712.0
96.10	7052.0
97.10	259.0
103.90	478.0
104.80	184.0
105.90	481.0
106.90	124.0
112.90	128.0
115.00	115.0
115.90	381.0
116.90	640.0
117.90	314.0
118.90	498.0
127.90	384.0
128.90	173.0
129.90	339.0
130.80	171.0
134.90	196.0
136.90	180.0
140.90	929.0
141.90	128.0
142.90	1147.0
145.00	114.0
145.90	127.0
147.90	208.0
148.90	112.0
149.80	118.0
154.90	206.0
157.00	159.0
161.00	121.0
174.00	68128.0
175.00	5810.0
176.00	66664.0
177.00	4783.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.10	1042.0
37.00	5819.0
38.00	4739.0
39.00	2111.0
40.00	290.0
41.00	273.0
42.10	161.0
43.00	307.0
44.00	1535.0
45.00	1059.0
45.80	137.0
47.00	1371.0
48.10	608.0
49.00	4946.0
50.00	21416.0
51.00	6650.0
52.00	342.0
55.00	472.0
56.00	1774.0
57.00	3029.0
58.10	159.0
60.00	1231.0
61.00	5417.0
62.00	5604.0
63.00	4039.0
64.00	379.0
66.90	400.0
68.00	11728.0
69.00	11894.0
70.00	906.0
71.00	129.0
72.00	652.0
73.00	4997.0
74.00	19392.0
75.10	58648.0
76.00	4839.0
77.00	764.0
77.80	477.0
78.90	3329.0
79.90	982.0
81.00	3241.0
81.90	705.0
83.10	197.0
86.10	241.0
87.00	4831.0
88.00	3969.0
90.90	508.0
92.10	3150.0
93.00	4788.0
94.10	13061.0
95.10	110752.0
96.10	7817.0
97.00	230.0
103.90	529.0
104.90	214.0
105.90	493.0
106.90	142.0
110.90	139.0
112.90	151.0
115.00	114.0
115.90	446.0
116.90	678.0
118.00	367.0
118.90	568.0
127.90	387.0
128.90	219.0
129.90	364.0
130.90	167.0
134.90	196.0
136.90	249.0
140.90	1052.0
141.90	129.0
142.90	1229.0
144.90	118.0
145.90	138.0
147.90	239.0
148.90	114.0
149.80	128.0
155.00	203.0
157.00	189.0
159.00	108.0
160.90	135.0
171.50	102.0
174.00	76896.0
175.00	6401.0
176.00	74784.0
177.00	5201.0
177.90	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.00	978.0
37.00	5573.0
38.10	4498.0
39.00	2023.0
40.00	298.0
41.10	252.0
42.10	155.0
42.90	339.0
44.00	1438.0
45.00	1037.0
45.90	131.0
47.00	1237.0
48.00	630.0
49.00	4762.0
50.00	21000.0
51.00	6484.0
52.00	298.0
55.00	469.0
56.00	1726.0
57.00	2928.0
58.10	198.0
60.00	1272.0
61.00	5214.0
62.00	5491.0
63.00	3912.0
64.00	397.0
66.90	398.0
68.00	11052.0
69.10	11544.0
70.00	816.0
71.00	119.0
72.00	657.0
73.00	4993.0
74.00	18912.0
75.10	56968.0
76.10	4743.0
77.00	739.0
77.80	492.0
78.90	3218.0
79.90	939.0
81.00	3202.0
81.90	700.0
83.10	177.0
86.00	252.0
87.00	4468.0
88.00	3902.0
90.90	511.0
92.00	3151.0
93.00	4745.0
94.10	12587.0
95.10	108496.0
96.10	7632.0
97.00	219.0
103.90	528.0
104.90	236.0
105.90	452.0
106.90	139.0
110.90	167.0
112.80	152.0
115.20	140.0
115.90	468.0
116.90	654.0
118.00	387.0
118.90	580.0
127.90	365.0
128.90	231.0
129.80	368.0
131.00	185.0
134.90	209.0
136.90	275.0
140.90	1089.0
141.90	105.0
142.90	1175.0
144.90	116.0
145.90	141.0
147.90	244.0
149.80	125.0
155.00	212.0
156.90	160.0
159.10	119.0
161.00	137.0
171.80	132.0
174.00	78272.0
175.10	6401.0
176.00	75720.0
177.00	5065.0
178.00	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288