


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082518\
Data File : VV007194.D
Acq On : 25 Aug 2018 10:33
Operator : SY/MD
Sample : BFB65
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082418WMA.M
Title : VOC Analysis
Last Update : Mon Aug 27 04:49:25 2018

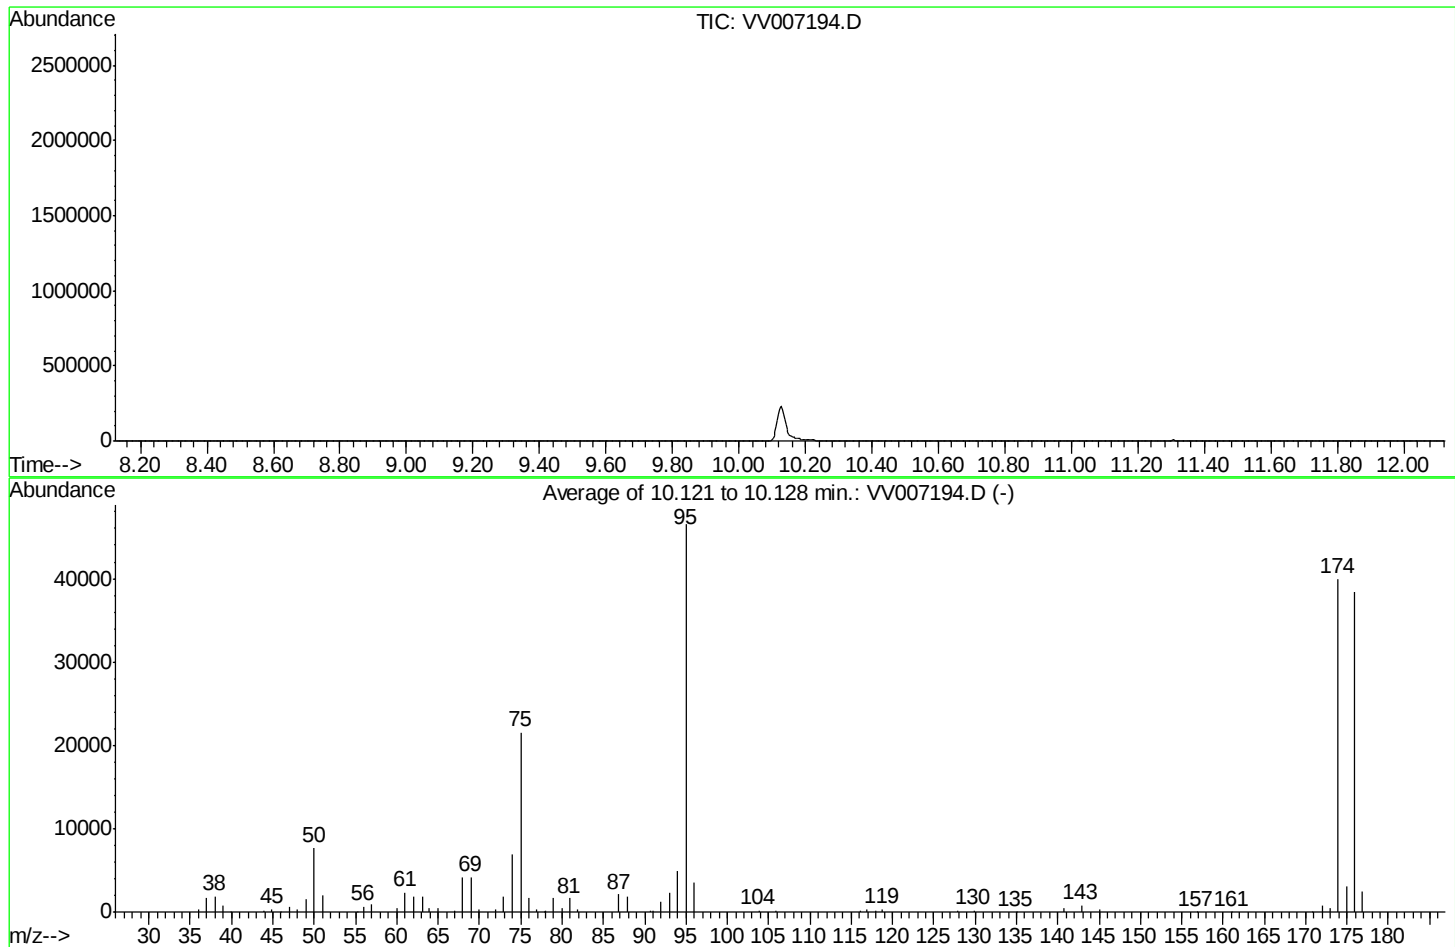

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	7681	PASS
75	95	30	80	46.3	21533	PASS
95	95	100	100	100.0	46506	PASS
96	95	5	9	7.5	3470	PASS
173	174	0.00	2	1.3	514	PASS
174	95	50	120	85.9	39954	PASS
175	174	5	9	7.7	3084	PASS
176	174	95	101	96.2	38432	PASS
177	176	5	9	6.3	2421	PASS

Scan 2860 (10.086 min): VV007194.D
BFB65

m/z	Abundance
39.90	500.0
43.90	1024.0
206.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	328.0
37.00	1800.0
38.00	1921.0
39.00	789.0
39.90	500.0
44.00	1112.0
44.90	325.0
46.90	719.0
47.90	350.0
49.00	1373.0
50.00	7812.0
51.00	2194.0
56.00	648.0
57.00	1062.0
60.00	355.0
61.00	2195.0
62.00	1947.0
63.00	1750.0
63.90	378.0
65.10	416.0
67.00	139.0
68.00	3876.0
69.00	4117.0
70.00	347.0
71.90	323.0
73.00	1726.0
74.00	6692.0
75.00	20480.0
76.00	1734.0
76.90	316.0
77.80	165.0
78.90	1475.0
80.00	488.0
80.90	1673.0
81.90	335.0
86.90	2045.0
88.00	1836.0
90.80	143.0
92.00	1043.0
93.00	2268.0
94.00	5031.0
95.00	44088.0
96.00	3407.0
103.90	199.0
105.90	125.0
116.80	330.0
117.90	174.0
118.80	353.0
127.80	233.0
129.80	196.0
140.80	384.0
142.90	801.0
145.00	212.0
172.00	633.0
172.80	509.0
173.90	36408.0
174.90	3105.0
175.90	35512.0
176.90	2334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	361.0
37.00	1791.0
38.00	1902.0
39.00	816.0
39.90	492.0
43.90	1225.0
44.90	318.0
46.00	110.0
47.00	578.0
47.90	315.0
49.00	1509.0
50.00	7817.0
51.00	2065.0
56.00	672.0
57.00	1016.0
60.00	411.0
61.00	2419.0
62.00	1935.0
63.10	1860.0
63.90	433.0
65.00	419.0
67.10	141.0
68.00	4246.0
69.00	4301.0
70.00	309.0
71.90	360.0
72.90	1848.0
74.00	7172.0
75.00	22280.0
76.00	1740.0
76.90	331.0
78.00	193.0
78.90	1709.0
79.90	552.0
80.90	1693.0
81.80	344.0
86.90	2237.0
88.00	1844.0
91.00	127.0
92.00	1206.0
92.90	2306.0
94.00	5047.0
95.00	47800.0
96.00	3580.0
103.80	232.0
105.80	159.0
116.10	128.0
116.80	340.0
117.90	185.0
118.80	381.0
127.80	198.0
129.80	205.0
135.00	101.0
140.80	434.0
142.90	842.0
145.00	368.0
171.90	781.0
172.90	494.0
173.90	41160.0
174.90	3230.0
175.90	39656.0
176.90	2508.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	365.0
37.00	1669.0
38.00	1778.0
39.00	716.0
39.90	570.0
44.00	1390.0
44.90	342.0
46.00	127.0
47.10	427.0
47.90	257.0
48.90	1561.0
50.00	7414.0
51.00	1896.0
55.20	102.0
56.00	600.0
57.00	880.0
60.00	502.0
61.00	2315.0
62.00	1868.0
63.10	1849.0
63.90	422.0
64.90	490.0
67.10	146.0
68.00	4246.0
69.00	4131.0
70.00	297.0
71.90	354.0
72.90	1794.0
74.00	7001.0
75.00	21840.0
76.00	1774.0
77.00	346.0
78.00	227.0
78.90	1786.0
79.90	535.0
80.90	1614.0
81.90	281.0
86.90	2092.0
87.90	1947.0
90.70	114.0
91.10	123.0
92.00	1314.0
92.90	2267.0
94.00	4844.0
95.00	47632.0
96.00	3424.0
103.80	227.0
105.80	205.0
116.10	171.0
116.80	319.0
117.90	174.0
118.80	344.0
127.90	136.0
129.90	212.0
140.80	426.0
142.80	810.0
145.00	470.0
156.80	110.0
161.10	115.0
170.80	110.0
172.00	866.0
173.00	540.0
173.90	42296.0
174.90	2919.0
175.90	40128.0
176.90	2423.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65