


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082520\
 Data File : VV018088.D
 Acq On : 25 Aug 2020 09:13
 Operator : SY/MD
 Sample : BFB81
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 26 02:11:17 2020

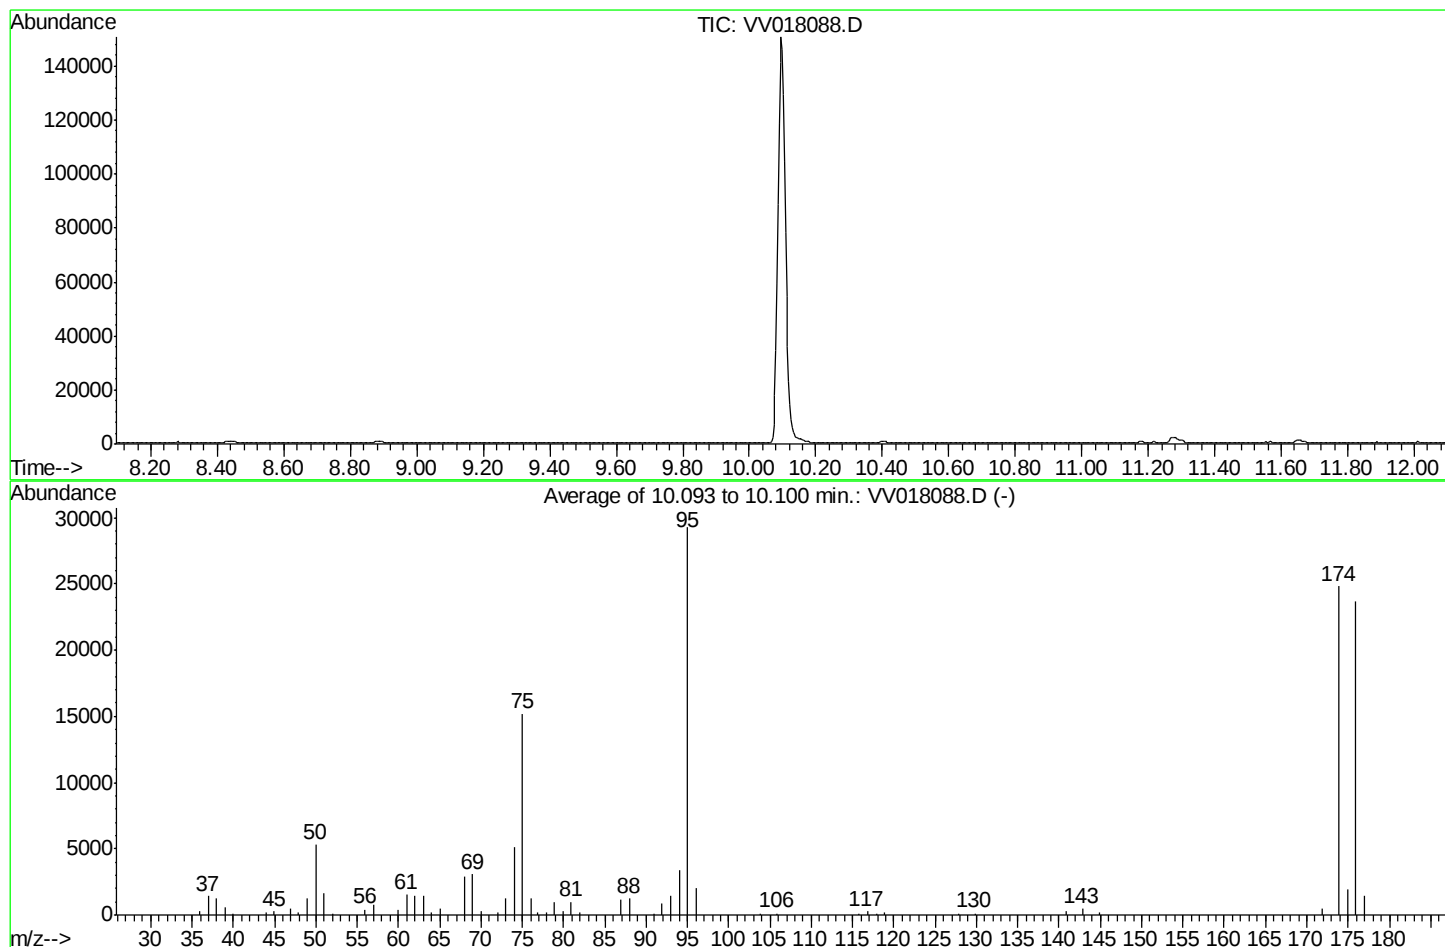

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5295	PASS
75	95	30	80	51.9	15178	PASS
95	95	100	100	100.0	29272	PASS
96	95	5	9	6.9	2022	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	24810	PASS
175	174	5	9	7.8	1933	PASS
176	174	95	101	95.5	23698	PASS
177	176	5	9	6.2	1466	PASS

m/z	Abundance
35.90	285.0
37.00	1353.0
38.00	1187.0
38.90	623.0
39.90	207.0
43.90	533.0
44.90	285.0
47.00	407.0
47.90	176.0
49.00	1194.0
50.00	5323.0
51.00	1659.0
52.00	140.0
55.90	391.0
57.00	730.0
59.90	362.0
61.00	1503.0
62.00	1403.0
63.00	1481.0
64.00	200.0
65.00	404.0
68.00	2792.0
69.00	3111.0
70.00	258.0
72.10	169.0
73.00	1300.0
74.00	4862.0
75.00	14745.0
76.00	1261.0
76.90	193.0
77.90	143.0
78.90	918.0
79.90	298.0
80.90	988.0
81.90	224.0
86.90	1199.0
87.90	1180.0
90.90	107.0
91.90	845.0
93.00	1477.0
94.00	3263.0
95.00	28720.0
96.00	1931.0
103.90	123.0
105.90	116.0
115.80	122.0
116.80	272.0
117.90	138.0
118.90	197.0
129.80	133.0
140.80	241.0
142.80	434.0
144.90	158.0
171.90	423.0
173.90	23352.0
174.90	1877.0
175.90	22472.0
176.90	1342.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	293.0
37.00	1476.0
38.00	1233.0
38.90	605.0
39.90	203.0
44.00	601.0
45.00	297.0
47.00	471.0
47.90	175.0
49.00	1275.0
50.00	5428.0
51.00	1666.0
52.00	149.0
56.00	426.0
57.00	794.0
59.90	372.0
61.00	1594.0
62.00	1491.0
63.00	1476.0
64.00	185.0
65.00	462.0
68.00	2976.0
69.00	3152.0
70.00	266.0
72.10	149.0
73.00	1314.0
74.00	5279.0
75.00	15713.0
76.00	1225.0
76.90	245.0
77.90	170.0
78.90	1038.0
79.90	306.0
80.90	1059.0
81.90	251.0
86.90	1234.0
87.90	1291.0
90.90	102.0
91.90	873.0
93.00	1527.0
94.00	3517.0
95.00	30096.0
96.00	2082.0
103.80	136.0
105.90	131.0
115.80	155.0
116.80	264.0
117.90	137.0
118.90	191.0
127.80	102.0
129.90	150.0
140.80	272.0
142.90	462.0
144.90	169.0
171.90	473.0
173.90	25640.0
174.90	1976.0
175.90	24544.0
176.90	1505.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	277.0
37.00	1402.0
38.00	1234.0
39.00	520.0
39.90	211.0
44.00	608.0
45.00	273.0
47.00	443.0
47.90	165.0
49.00	1259.0
50.00	5136.0
51.00	1519.0
52.00	133.0
56.00	412.0
57.00	801.0
60.00	352.0
61.00	1439.0
62.00	1452.0
63.00	1284.0
64.10	173.0
65.00	457.0
68.00	2894.0
69.00	2906.0
70.00	262.0
72.10	135.0
73.00	1212.0
74.00	5146.0
75.00	15078.0
76.00	1212.0
76.90	262.0
77.90	157.0
78.90	1090.0
79.90	308.0
80.90	1001.0
81.90	252.0
86.90	1152.0
88.00	1234.0
92.00	864.0
93.00	1389.0
94.00	3496.0
95.00	29000.0
96.00	2053.0
103.80	116.0
105.90	139.0
115.80	152.0
116.80	235.0
117.90	112.0
118.90	173.0
127.80	107.0
129.90	135.0
140.80	283.0
142.90	463.0
144.90	151.0
171.90	490.0
173.90	25440.0
174.90	1946.0
175.90	24080.0
176.90	1552.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Scan 2790 (10.061 min): VV018088.D
BFB81

m/z	Abundance
39.90	134.0
44.00	398.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81