


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082521\
 Data File : VV021938.D
 Acq On : 25 Aug 2021 09:17
 Operator : SY/MD
 Sample : BFB221
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB221

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 26 05:17:05 2021

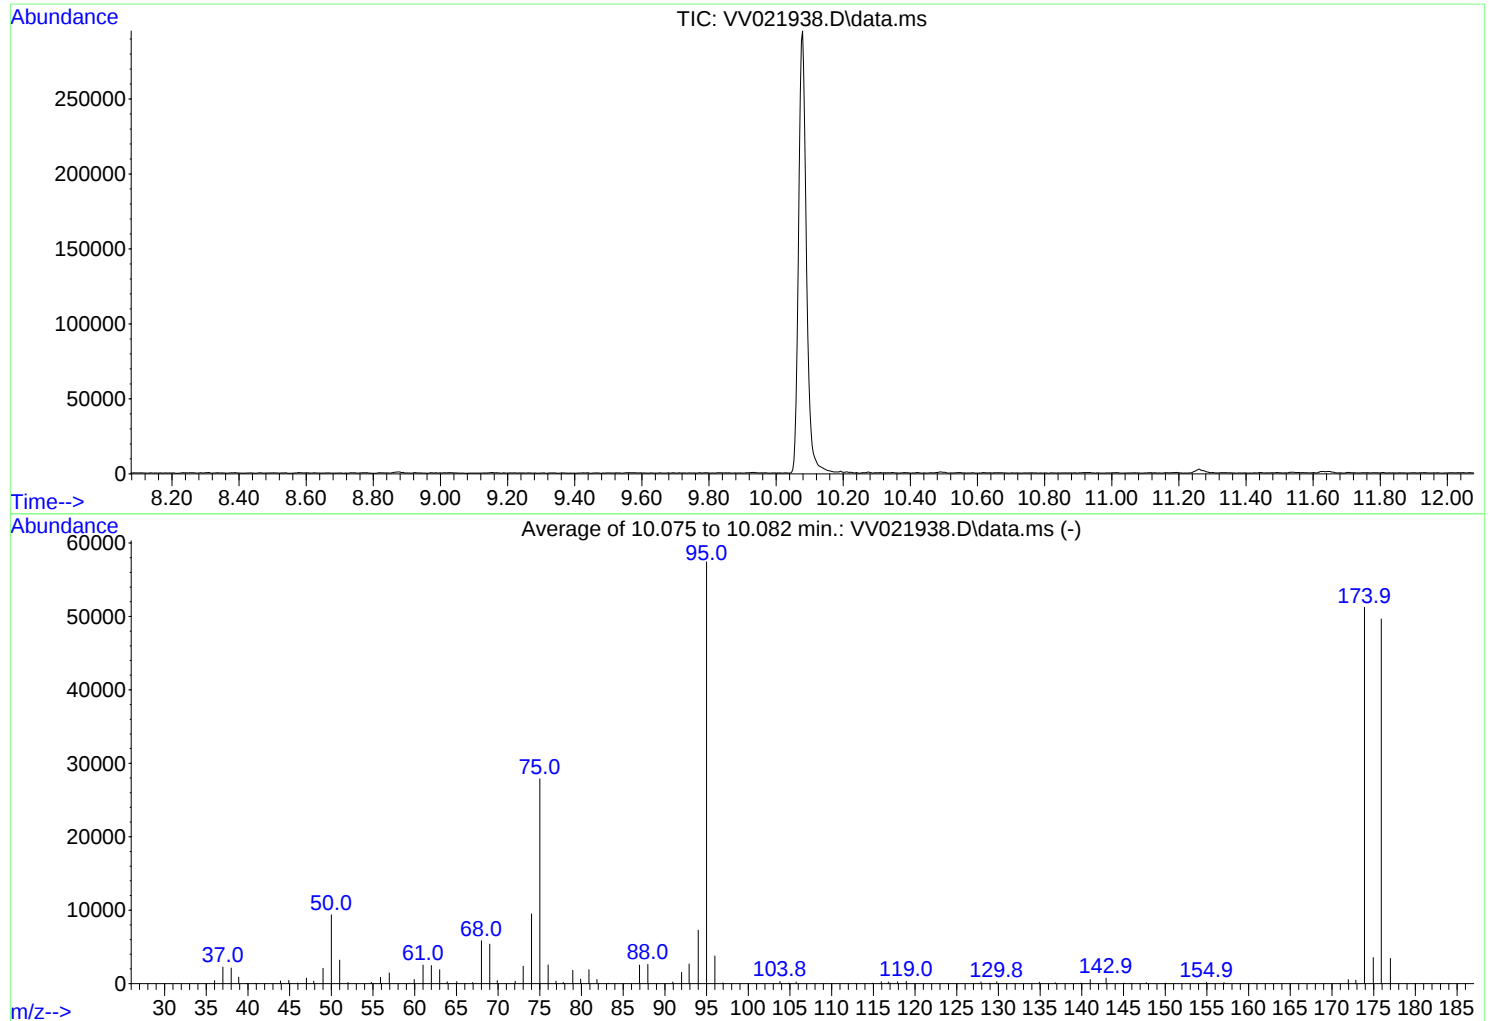

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9377	PASS
75	95	30	80	48.6	27899	PASS
95	95	100	100	100.0	57437	PASS
96	95	5	9	6.6	3766	PASS
173	174	0.00	2	0.9	480	PASS
174	95	50	120	89.2	51243	PASS
175	174	5	9	6.9	3554	PASS
176	174	95	105	96.9	49648	PASS
177	176	5	10	6.9	3422	PASS

Scan 2799 (10.040 min): VV021938.D\data.ms
BFB221

m/z	Abundance
39.80	202.0
43.90	306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	418.0
37.00	2331.0
38.00	2212.0
38.90	928.0
39.90	209.0
43.90	673.0
44.90	443.0
46.00	110.0
47.00	776.0
47.90	357.0
49.00	2179.0
50.00	9697.0
51.00	3282.0
52.00	176.0
54.80	177.0
55.90	873.0
57.00	1519.0
59.90	597.0
61.00	2607.0
62.00	2570.0
63.00	1915.0
63.90	271.0
65.00	301.0
66.90	157.0
68.00	6016.0
69.00	5673.0
69.90	398.0
72.00	338.0
73.00	2446.0
74.00	9862.0
75.00	28760.0
76.00	2633.0
77.00	333.0
77.80	174.0
78.90	1855.0
79.90	630.0
80.90	1950.0
81.80	614.0
83.20	102.0
86.90	2639.0
87.90	2651.0
90.90	216.0
92.00	1581.0
92.90	2857.0
94.00	7568.0
95.00	59424.0
96.00	3923.0
97.00	124.0
103.80	324.0
104.90	115.0
105.70	235.0
112.90	101.0
114.90	109.0
116.00	275.0
116.80	314.0
117.90	272.0
119.00	322.0
127.90	259.0
128.90	126.0
129.80	279.0
134.90	207.0
136.80	127.0
139.90	111.0
141.00	556.0
142.90	798.0
145.10	101.0
145.90	101.0
147.70	146.0
150.00	108.0
154.90	213.0
157.10	166.0
171.90	556.0
172.80	492.0
173.90	53016.0
174.90	3609.0
175.90	51216.0
177.00	3546.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	439.0
37.00	2348.0
38.00	2158.0
38.90	906.0
39.90	195.0
43.90	696.0
44.90	461.0
47.00	841.0
47.90	361.0
49.00	2125.0
50.00	9904.0
51.00	3400.0
52.00	146.0
54.80	199.0
55.90	903.0
56.90	1492.0
59.90	566.0
61.00	2691.0
62.00	2443.0
63.00	2101.0
63.90	215.0
65.00	323.0
67.00	179.0
68.00	6188.0
69.00	5388.0
69.90	421.0
72.00	332.0
73.00	2442.0
74.00	9639.0
75.00	28536.0
76.00	2596.0
76.90	423.0
77.70	213.0
79.00	1852.0
79.90	592.0
80.90	1921.0
81.90	611.0
83.20	108.0
87.00	2445.0
88.00	2773.0
90.90	228.0
92.00	1529.0
92.90	2658.0
94.00	7165.0
95.00	58144.0
96.00	3916.0
96.90	109.0
103.80	307.0
104.80	133.0
105.90	235.0
116.00	288.0
116.80	391.0
117.90	312.0
119.00	352.0
127.90	238.0
129.80	286.0
134.90	194.0
136.80	101.0
139.90	123.0
141.00	549.0
142.90	753.0
145.90	115.0
147.80	147.0
150.00	118.0
154.90	172.0
157.10	138.0
160.70	117.0
172.00	530.0
172.90	441.0
173.90	51160.0
174.90	3693.0
175.90	49000.0
177.00	3628.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	398.0
37.00	2125.0
38.00	2033.0
38.90	855.0
39.90	233.0
40.90	105.0
43.90	636.0
44.90	404.0
45.90	146.0
47.00	653.0
47.90	310.0
49.00	2003.0
50.00	8530.0
51.00	2904.0
52.00	157.0
54.80	130.0
55.90	753.0
57.00	1391.0
60.00	543.0
61.00	2299.0
62.00	2377.0
63.00	1671.0
63.90	272.0
65.10	249.0
66.00	121.0
67.00	147.0
68.00	5316.0
69.00	5084.0
69.90	434.0
72.10	306.0
73.00	2224.0
74.00	8968.0
75.00	26400.0
76.00	2431.0
77.00	300.0
77.90	161.0
78.90	1706.0
79.90	601.0
80.90	1823.0
81.80	512.0
86.90	2490.0
87.90	2443.0
91.00	215.0
92.00	1500.0
92.90	2548.0
94.00	7119.0
95.00	54744.0
96.00	3459.0
97.00	128.0
103.80	288.0
105.70	223.0
114.90	119.0
115.90	231.0
117.00	271.0
117.90	198.0
118.80	290.0
127.90	246.0
129.00	127.0
129.80	254.0
134.90	157.0
136.80	157.0
141.00	521.0
142.90	715.0
145.10	114.0
147.70	132.0
155.00	194.0
157.00	143.0
171.90	548.0
172.80	507.0
173.90	49552.0
175.00	3361.0
175.90	48728.0
177.00	3092.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221