




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027500.D
 Acq On : 25 Aug 2022 17:24
 Operator : SY/MD
 Sample : N4370-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E83

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/27/2022
 Supervised By :Semsettin Yesilyurt 08/27/2022

Quant Time: Aug 26 01:00:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 26 00:58:54 2022
 Response via : Initial Calibration

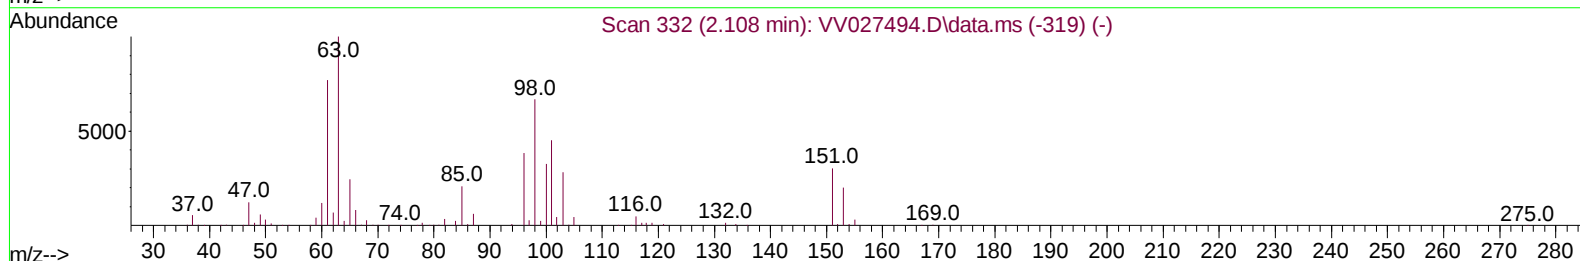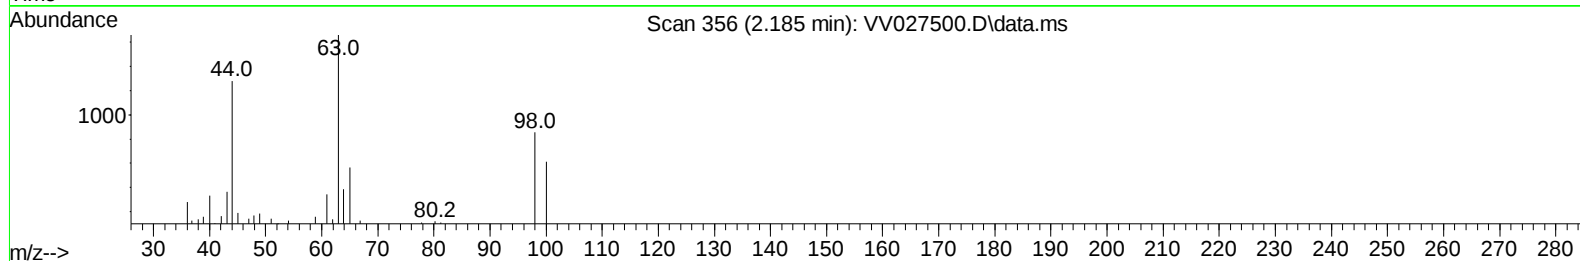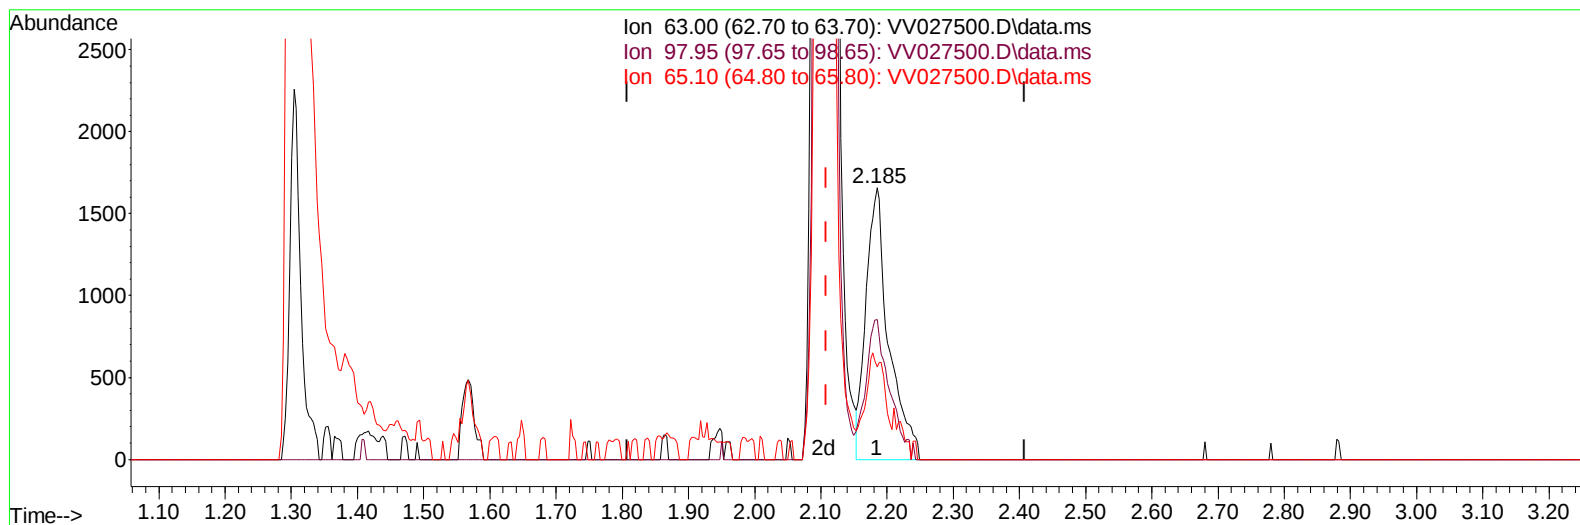

TIC: VV027500.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.185min (+ 0.077) 0.23 ug/L

response 3961

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	54.43
65.10	22.40	22.60
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027500.D
 Acq On : 25 Aug 2022 17:24
 Operator : SY/MD
 Sample : N4370-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E83

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:00:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 26 00:58:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/27/2022
 Supervised By :Semsettin Yesilyurt 08/27/2022

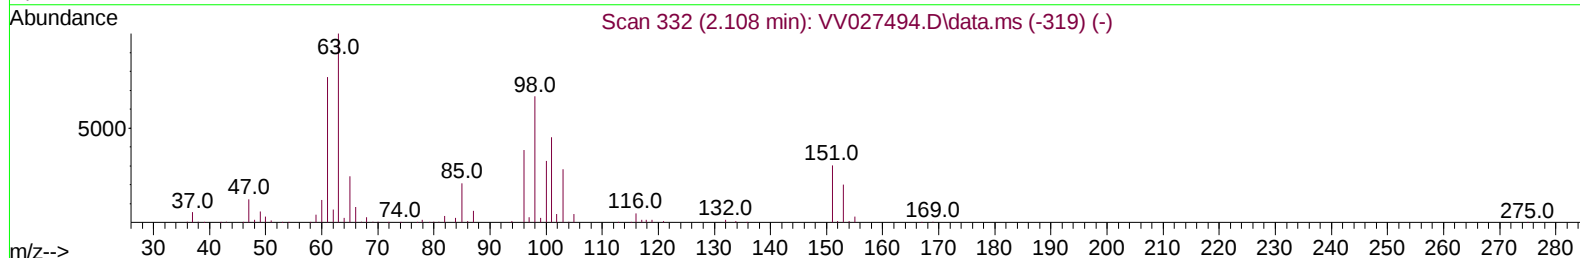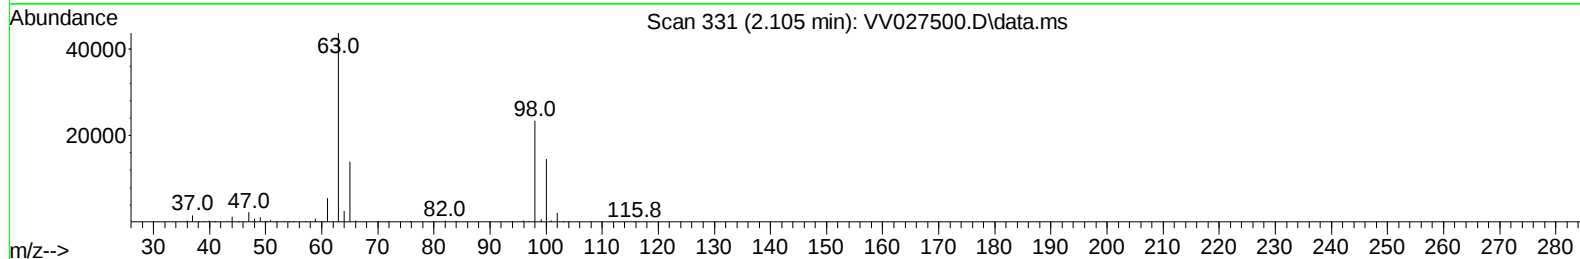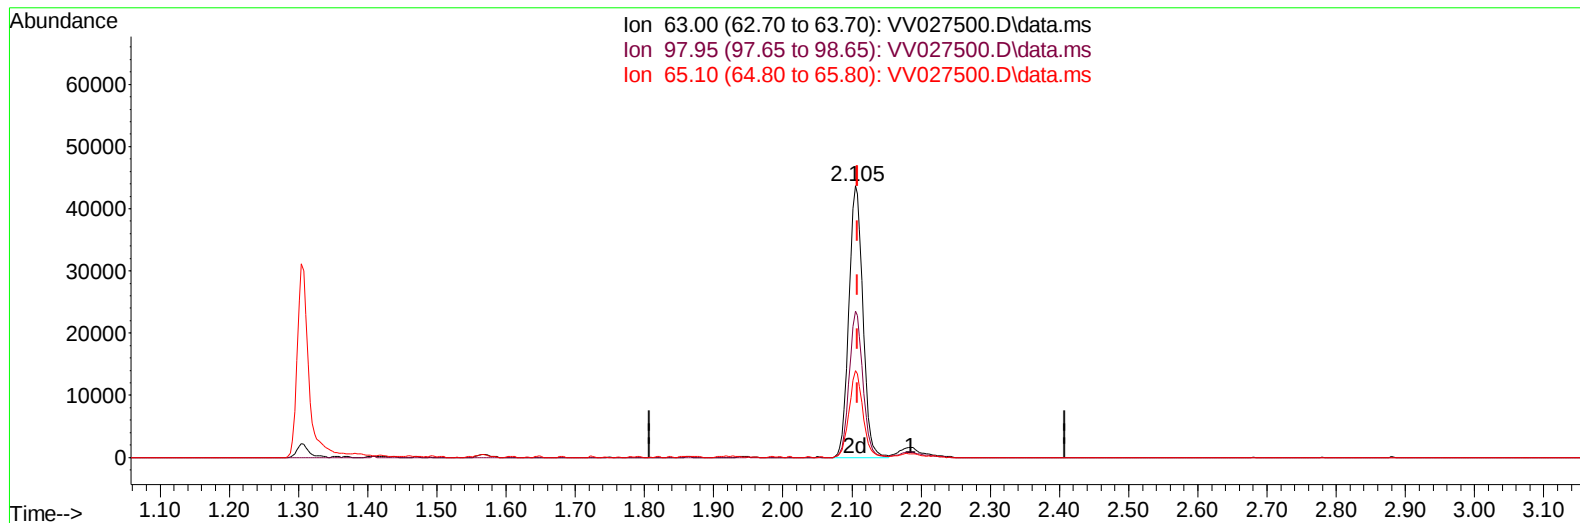

TIC: VV027500.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (-0.003) 3.60 ug/L m

response 62122

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	3.47#
65.10	22.40	1.44#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027500.D
 Acq On : 25 Aug 2022 17:24
 Operator : SY/MD
 Sample : N4370-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E83

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/27/2022
 Supervised By :Semsettin Yesilyurt 08/27/2022

Quant Time: Aug 26 01:00:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 26 00:58:54 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		104003	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		104618	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		46904	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		36478	4.928	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.600%	
7) Chloroethane-d5	1.568	69		31074	5.736	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.800%	
11) 1,1-Dichloroethene-d2	2.105	63		62122m	3.599	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%	
20) 2-Butanone-d5	3.899	46		44155	47.934	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.860%	
24) Chloroform-d	4.349	84		72667	4.910	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%	
26) 1,2-Dichloroethane-d4	5.034	65		30859	4.820	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.400%	
32) Benzene-d6	5.050	84		129098	4.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%	
36) 1,2-Dichloropropane-d6	6.069	67		40268	4.780	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.600%	
41) Toluene-d8	7.317	98		103967	3.974	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%	
43) trans-1,3-Dichloroprop...	7.628	79		12432	4.310	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%	
46) 2-Hexanone-d5	8.091	63		43329	45.631	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		25863	4.821	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152		35383	5.089	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027500.D
Acq On : 25 Aug 2022 17:24
Operator : SY/MD
Sample : N4370-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E83

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:00:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 26 00:58:54 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/27/2022
Supervised By :Semsettin Yesilyurt 08/27/2022

