




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027516.D
Acq On : 26 Aug 2022 00:23
Operator : SY/MD
Sample : N4367-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F19

Manual IntegrationsAPPROVED

Quant Time: Aug 26 02:03:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 26 01:50:00 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/27/2022
Supervised By :Semsettin Yesilyurt 08/27/2022

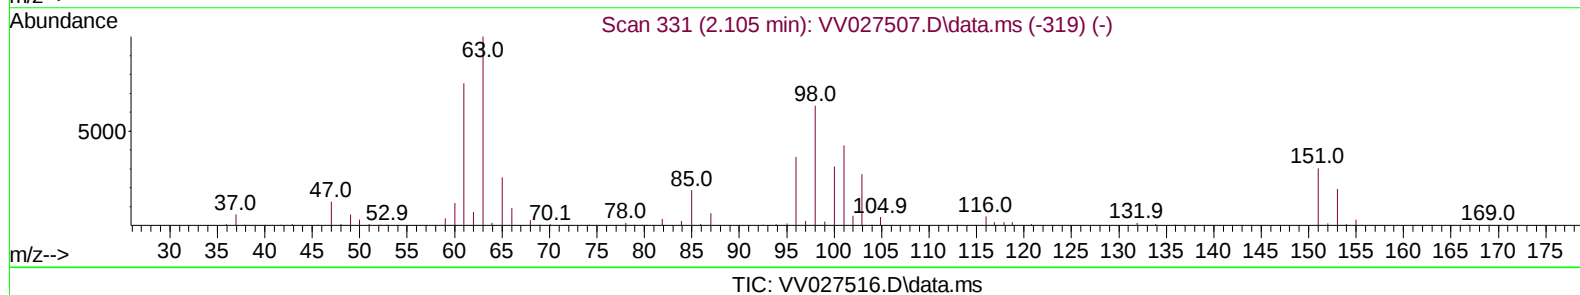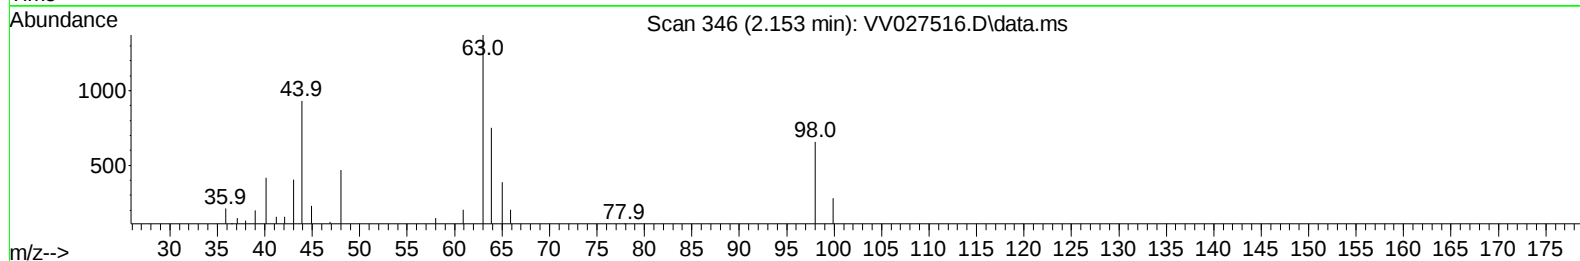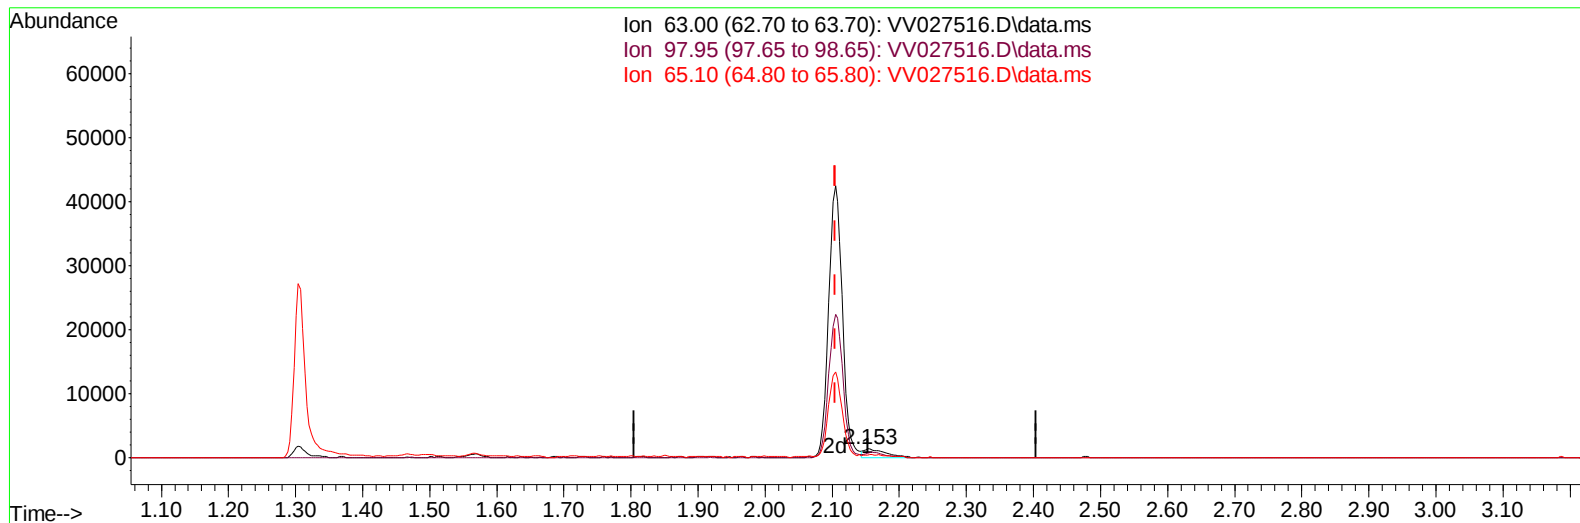

(11) 1,1-Dichloroethene-d2 (S)

2.153min (+ 0.048) 0.16 ug/L

response 3003

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	54.81
65.10	22.40	18.61
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027516.D
Acq On : 26 Aug 2022 00:23
Operator : SY/MD
Sample : N4367-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F19

Manual IntegrationsAPPROVED

Quant Time: Aug 26 02:03:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 26 01:50:00 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/27/2022
Supervised By :Semsettin Yesilyurt 08/27/2022

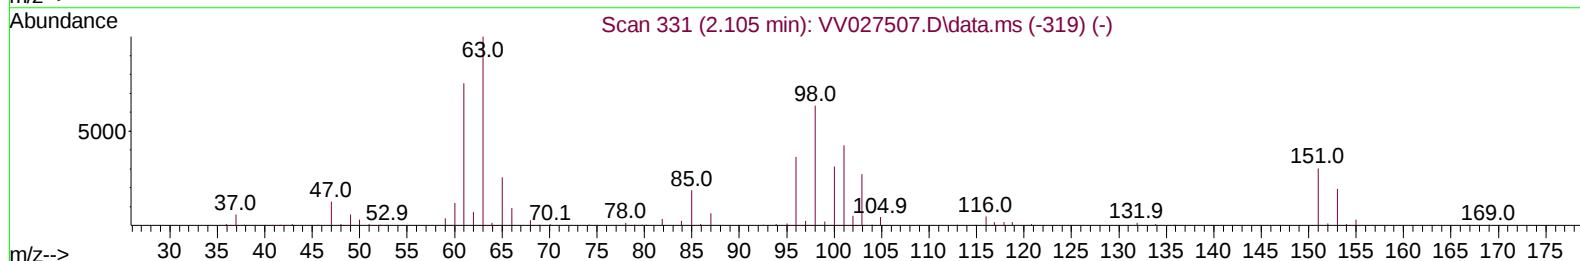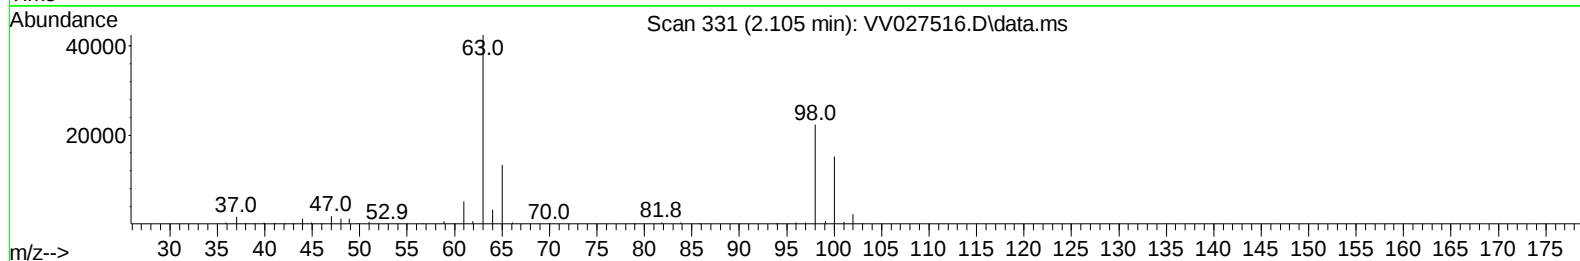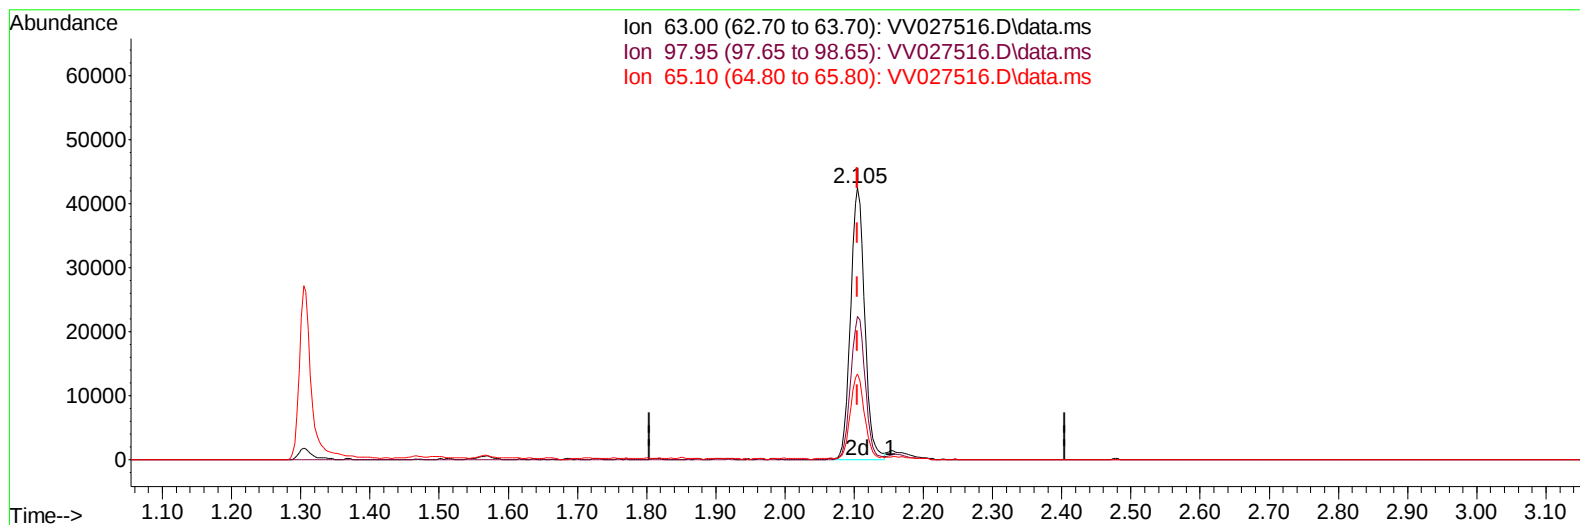

TIC: VV027516.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (+ 0.000) 3.20 ug/L m

response 60605

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	2.72#
65.10	22.40	0.92#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027516.D
 Acq On : 26 Aug 2022 00:23
 Operator : SY/MD
 Sample : N4367-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F19

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/27/2022
 Supervised By :Semsettin Yesilyurt 08/27/2022

Quant Time: Aug 26 02:03:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 26 01:50:00 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		114117	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		113827	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		50342	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		33256	4.095	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.800%	
7) Chloroethane-d5	1.565	69		31250	5.257	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.200%	
11) 1,1-Dichloroethene-d2	2.105	63		60605m	3.200	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.000%	
20) 2-Butanone-d5	3.899	46		59548	58.915	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.820%	
24) Chloroform-d	4.346	84		71639	4.411	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%	
26) 1,2-Dichloroethane-d4	5.031	65		32946	4.689	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%	
32) Benzene-d6	5.047	84		123928	3.931	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.600%	
36) 1,2-Dichloropropane-d6	6.069	67		38763	4.229	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.600%	
41) Toluene-d8	7.317	98		97503	3.425	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.600%#	
43) trans-1,3-Dichloroprop...	7.629	79		8422	2.683	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	53.600%#	
46) 2-Hexanone-d5	8.088	63		41817	40.476	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.960%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		24043	4.119	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		33060	4.430	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.600%	
Target Compounds							
47) Tetrachloroethene	7.973	164		57594	7.423	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027516.D
Acq On : 26 Aug 2022 00:23
Operator : SY/MD
Sample : N4367-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F19

Manual IntegrationsAPPROVED

Quant Time: Aug 26 02:03:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 26 01:50:00 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/27/2022
Supervised By :Semsettin Yesilyurt 08/27/2022

